

2/10/2204

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/18/2019 15:02

Test: Reactive
Total CN

Sample Id	Result <u>ug/l</u>	Dil. 1 +	Response	Errors
ICV1	93.979	0.0	0.091	
ICB1	-0.586	0.0	0.004	
CCV1	245.411	0.0	0.229	
CCB1	-0.631	0.0	0.004	
PB119021BL	-0.871	0.0	0.004	
K2193-08	-0.612	0.0	0.004	
K2193-08DUP	-0.923	0.0	0.004	
K2193-10	-1.044	0.0	0.004	
K2193-12	-1.202	0.0	0.004	
K2198-06	-1.030	0.0	0.004	
K2453-02	-0.900	0.0	0.004	
CCV2	253.125	0.0	0.236	
CCB2	-1.011	0.0	0.004	

N 13
Mean 44.900
SD 94.3974
CV% 210.24

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/18/2019 13:38


Test Total CN

Accepted 4/18/2019 13:38

Factor 1095
Bias 0.005

Coeff. of det. 0.999961

Errors

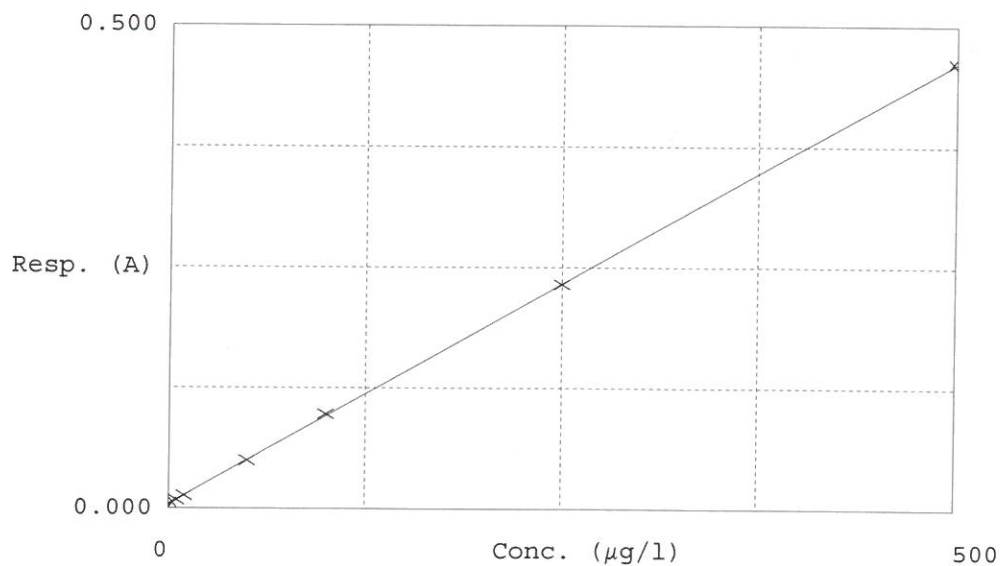

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.006	1.1452	0.0000	
2	5.0PPBCN	0.009	4.0964	5.0000	
3	10PPBCN	0.013	9.1936	10.0000	
4	50PPBCN	0.050	49.2754	50.0000	
5	100PPBCN	0.098	101.9973	100.0000	
6	250PPBCN	0.233	249.1878	250.0000	
7	500PPBCN	0.462	500.1043	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Thu Apr 18 14:58:24 2019

Thu Apr 18 15:01:48 2019

AS

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	1.1452	µg/l	4/18/2019 13:14:33	
5.OPPBCN	A	Reactive CN	P	4.0964	µg/l	4/18/2019 13:14:34	
10PPBCN	A	Reactive CN	P	9.1936	µg/l	4/18/2019 13:14:35	
50PPBCN	A	Reactive CN	P	49.2754	µg/l	4/18/2019 13:14:36	
100PPBCN	A	Reactive CN	P	101.9973	µg/l	4/18/2019 13:14:37	
250PPBCN	A	Reactive CN	P	249.1878	µg/l	4/18/2019 13:14:38	
500PPBCN	A	Reactive CN	P	500.1043	µg/l	4/18/2019 13:14:39	
ICV1	S	Reactive CN	P	93.9792	µg/l	4/18/2019 14:58:24	
ICB1	S	Reactive CN	P	-0.5863	µg/l	4/18/2019 14:58:25	
CCV1	S	Reactive CN	P	245.4113	µg/l	4/18/2019 14:58:26	
CCB1	S	Reactive CN	P	-0.6309	µg/l	4/18/2019 14:58:27	
PB119021BL	S	Reactive CN	P	-0.8714	µg/l	4/18/2019 14:58:28	
K2193-08	S	Reactive CN	P	-0.6116	µg/l	4/18/2019 14:58:29	
K2193-08DUP	S	Reactive CN	P	-0.9226	µg/l	4/18/2019 14:58:30	
K2193-10	S	Reactive CN	P	-1.0445	µg/l	4/18/2019 14:58:31	
K2193-12	S	Reactive CN	P	-1.2023	µg/l	4/18/2019 14:58:32	
K2198-06	S	Reactive CN	P	-1.0296	µg/l	4/18/2019 14:58:33	
K2453-02	S	Reactive CN	P	-0.8997	µg/l	4/18/2019 14:58:34	
CCV2	S	Reactive CN	P	253.1248	µg/l	4/18/2019 15:01:47	
CCB2	S	Reactive CN	P	-1.0107	µg/l	4/18/2019 15:01:48	