

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/26/2019 7:09

Test: Reactive
Total CN

Sample Id	Result <u>ug/L</u>	Dil. 1 +	Response	Errors
ICV1	98.518	0.0	0.093	
ICB1	0.355	0.0	0.004	
CCV1	247.142	0.0	0.227	
CCB1	0.148	0.0	0.004	
PB119217BL	0.129	0.0	0.004	
K2203-18	0.100	0.0	0.004	
K2203-18DUP	-0.175	0.0	0.004	
K2544-02	0.010	0.0	0.004	
K2553-03	0.151	0.0	0.004	
K2553-06	0.123	0.0	0.004	
K2554-03	0.083	0.0	0.004	
PB119218BL	-0.334	0.0	0.004	
K2545-02	0.054	0.0	0.004	
K2545-02DUP	0.340	0.0	0.004	
CCV2	254.987	0.0	0.234	
CCB2	0.041	0.0	0.004	
K2203-20	-0.222	0.0	0.004	
CCV3	255.065	0.0	0.234	
CCB3	0.104	0.0	0.004	

N	19
Mean	45.085
SD	94.9389
CV%	210.58

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/25/2019 14:13


Test Total CN

Accepted 4/25/2019 14:13

Factor 1109
Bias 0.004

Coeff. of det. 0.999902

Errors

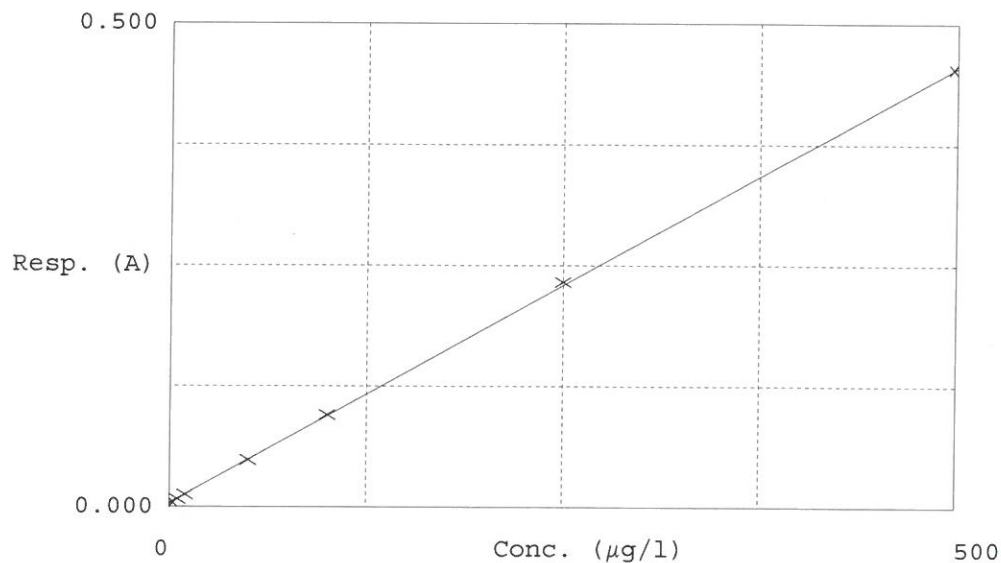

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.0038	0.0000	
2	5.0PPBCN	0.008	4.4615	5.0000	
3	10PPBCN	0.013	9.5120	10.0000	
4	50PPBCN	0.049	49.3021	50.0000	
5	100PPBCN	0.095	101.0337	100.0000	
6	250PPBCN	0.233	253.6325	250.0000	
7	500PPBCN	0.453	498.0620	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Thu Apr 25 16:10:12 2019

Thu Apr 25 16:16:59 2019

AS

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-1.0038	µg/l	4/25/2019 14:05:35	
5.OPPBCN	A	Reactive CN	P	4.4615	µg/l	4/25/2019 14:05:36	
10PPBCN	A	Reactive CN	P	9.512	µg/l	4/25/2019 14:05:37	
50PPBCN	A	Reactive CN	P	49.3021	µg/l	4/25/2019 14:05:38	
100PPBCN	A	Reactive CN	P	101.0337	µg/l	4/25/2019 14:05:39	
250PPBCN	A	Reactive CN	P	253.6325	µg/l	4/25/2019 14:05:40	
500PPBCN	A	Reactive CN	P	498.062	µg/l	4/25/2019 14:05:41	
ICV1	S	Reactive CN	P	98.5176	µg/l	4/25/2019 16:10:12	
ICB1	S	Reactive CN	P	0.3548	µg/l	4/25/2019 16:10:13	
CCV1	S	Reactive CN	P	247.1419	µg/l	4/25/2019 16:10:14	
CCB1	S	Reactive CN	P	0.1477	µg/l	4/25/2019 16:10:15	
PB119217BL	S	Reactive CN	P	0.1288	µg/l	4/25/2019 16:10:16	
K2203-18	S	Reactive CN	P	0.0999	µg/l	4/25/2019 16:10:17	
K2203-18DUP	S	Reactive CN	P	-0.1754	µg/l	4/25/2019 16:10:18	
K2544-02	S	Reactive CN	P	0.0105	µg/l	4/25/2019 16:10:19	
K2553-03	S	Reactive CN	P	0.1512	µg/l	4/25/2019 16:10:20	
K2553-06	S	Reactive CN	P	0.1227	µg/l	4/25/2019 16:10:21	
K2554-03	S	Reactive CN	P	0.0825	µg/l	4/25/2019 16:10:22	
PB119218BL	S	Reactive CN	P	-0.3343	µg/l	4/25/2019 16:16:51	
K2545-02	S	Reactive CN	P	0.0544	µg/l	4/25/2019 16:16:52	
K2545-02DUP	S	Reactive CN	P	0.3405	µg/l	4/25/2019 16:16:53	
CCV2	S	Reactive CN	P	254.9871	µg/l	4/25/2019 16:16:54	
CCB2	S	Reactive CN	P	0.0406	µg/l	4/25/2019 16:16:55	
K2203-20	S	Reactive CN	P	-0.2216	µg/l	4/25/2019 16:16:56	
CCV3	S	Reactive CN	P	255.0649	µg/l	4/25/2019 16:16:58	
CCB3	S	Reactive CN	P	0.1041	µg/l	4/25/2019 16:16:59	