

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/29/2019 15:19

Test: *Reactive*
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.497	0.0	0.096	
ICB1	0.780	0.0	0.004	
CCV1	244.167	0.0	0.236	
CCB1	0.312	0.0	0.004	
PB119294BL	0.266	0.0	0.004	
K2598-01	0.280	0.0	0.004	
K2598-01DUP	0.320	0.0	0.004	
CCV2	246.145	0.0	0.238	
CCB2	0.502	0.0	0.004	

N	9
Mean	65.585
SD	106.6529
CV%	162.62

AS

Aquakem v. 7.2AQ1

Results from time period:

Mon Apr 29 15:18:36 2019

Mon Apr 29 15:18:44 2019

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.5758	µg/l	4/29/2019 13:38:02	
5.OPPBCN	A	Reactive CN	P	4.8647	µg/l	4/29/2019 13:38:03	
10PPBCN	A	Reactive CN	P	9.8703	µg/l	4/29/2019 13:38:04	
50PPBCN	A	Reactive CN	P	48.5529	µg/l	4/29/2019 13:38:05	
100PPBCN	A	Reactive CN	P	100.9619	µg/l	4/29/2019 13:38:06	
250PPBCN	A	Reactive CN	P	250.4363	µg/l	4/29/2019 13:38:07	
500PPBCN	A	Reactive CN	P	499.7381	µg/l	4/29/2019 13:38:08	
ICV1	S	Reactive CN	P	97.4967	µg/l	4/29/2019 15:18:36	
ICB1	S	Reactive CN	P	0.7798	µg/l	4/29/2019 15:18:37	
CCV1	S	Reactive CN	P	244.1667	µg/l	4/29/2019 15:18:38	
CCB1	S	Reactive CN	P	0.3119	µg/l	4/29/2019 15:18:39	
PB119294BL	S	Reactive CN	P	0.2657	µg/l	4/29/2019 15:18:40	
K2598-01	S	Reactive CN	P	0.2798	µg/l	4/29/2019 15:18:41	
K2598-01DUP	S	Reactive CN	P	0.3201	µg/l	4/29/2019 15:18:42	
CCV2	S	Reactive CN	P	246.1451	µg/l	4/29/2019 15:18:43	
CCB2	S	Reactive CN	P	0.5021	µg/l	4/29/2019 15:18:44	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/29/2019 13:38


Test Total CN

Accepted 4/29/2019 13:38

Factor 1051
Bias 0.004

Coeff. of det. 0.999982

Errors

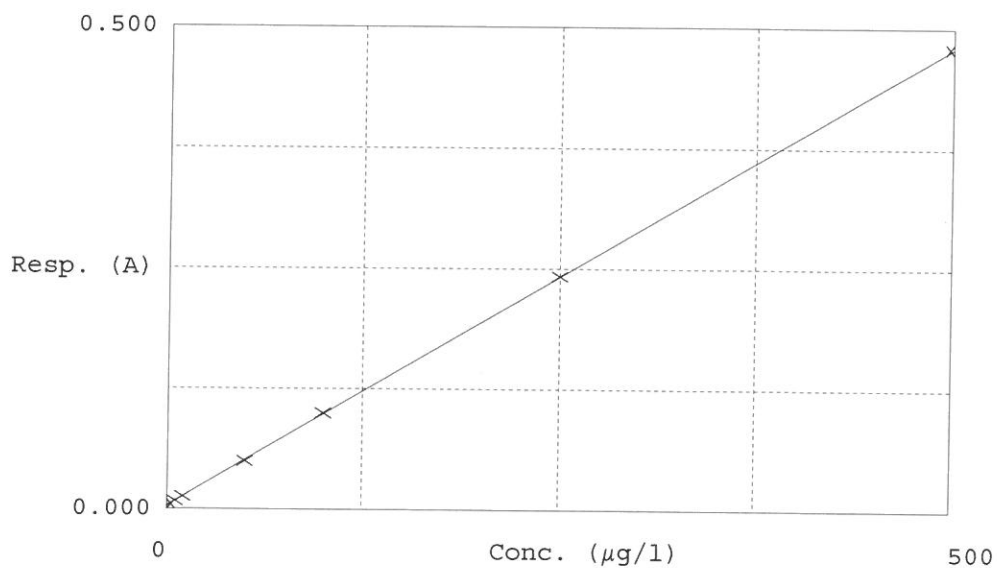

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.5758	0.0000	
2	5.0PPBCN	0.008	4.8647	5.0000	
3	10PPBCN	0.013	9.8703	10.0000	
4	50PPBCN	0.050	48.5529	50.0000	
5	100PPBCN	0.100	100.9619	100.0000	
6	250PPBCN	0.242	250.4363	250.0000	
7	500PPBCN	0.479	499.7381	500.0000	