

AB102546

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/3/2019 15:03

Test: Total CN

ug/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.760	0.0	0.098	
ICB1	0.589	0.0	0.004	
CCV1	244.619	0.0	0.244	
CCB1	0.388	0.0	0.004	
PB119450BL	0.462	0.0	0.004	
PB119450BS	98.935	0.0	0.101	
LOWPB119450	10.215	0.0	0.014	
HIGHPB119450	495.906	0.0	0.491	
K2635-01	1.821	0.0	0.006	
K2635-01DUP	1.509	0.0	0.005	
K2635-01MS	32.047	0.0	0.035	
K2635-01MSD	31.993	0.0	0.035	
K2635-03	1.271	0.0	0.005	
K2635-05	2.342	0.0	0.006	
CCV2	246.957	0.0	0.247	
CCB2	0.691	0.0	0.005	
K2635-07	1.215	0.0	0.005	
K2642-01	1.094	0.0	0.005	
K2647-01	3.087	0.0	0.007	
K2647-03	0.905	0.0	0.005	
K2667-01	2.520	0.0	0.006	
K2667-03	1.892	0.0	0.006	
K2668-01	0.464	0.0	0.004	
K2668-03	0.682	0.0	0.005	
K2668-05	0.782	0.0	0.005	
K2677-01	0.683	0.0	0.005	
CCV3	243.796	0.0	0.243	
CCB3	0.771	0.0	0.005	
K2678-01	3.714	0.0	0.007	
K2678-01DUP	3.539	0.0	0.007	
K2678-01MS	37.057	0.0	0.040	
K2678-01MSD	37.094	0.0	0.040	
CCV4	257.188	0.0	0.257	
CCB4	0.536	0.0	0.004	

N 34
Mean 54.780
SD 112.0375
CV% 204.52

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/3/2019 10:57


Test Total CN

Accepted 5/3/2019 10:57

Factor 1017
Bias 0.004

Coeff. of det. 0.999998

Errors

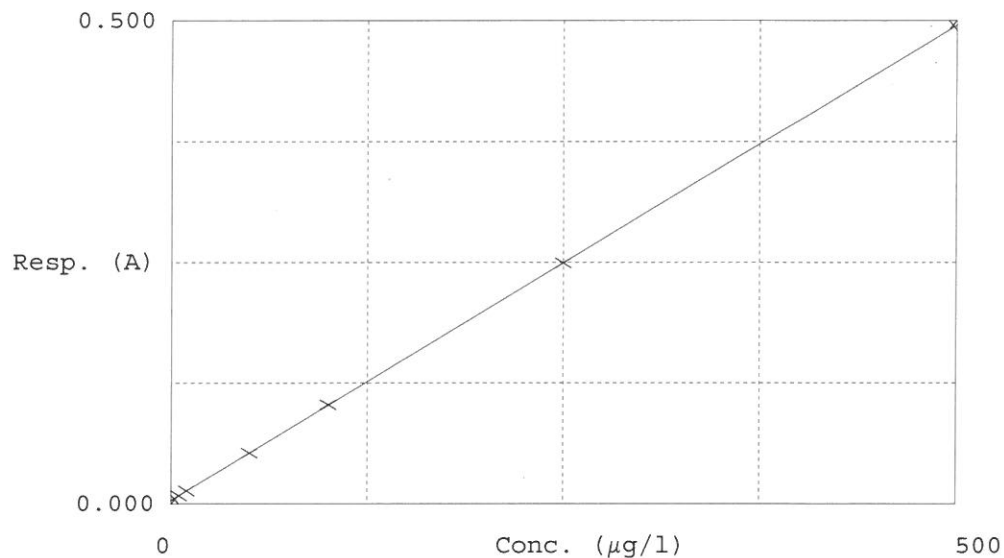

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.1048	0.0000	
2	5.0PPBCN	0.009	4.8530	5.0000	
3	10PPBCN	0.014	9.9176	10.0000	
4	50PPBCN	0.053	49.7769	50.0000	
5	100PPBCN	0.103	100.5138	100.0000	
6	250PPBCN	0.249	249.8226	250.0000	
7	500PPBCN	0.495	500.0113	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri May 03 14:39:50 2019

Fri May 03 15:00:17 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.1048	µg/l	5/3/2019 10:56:36	
5.OPPBCN	A	Total CN	P	4.853	µg/l	5/3/2019 10:56:37	
10PPBCN	A	Total CN	P	9.9176	µg/l	5/3/2019 10:56:38	
50PPBCN	A	Total CN	P	49.7769	µg/l	5/3/2019 10:56:39	
100PPBCN	A	Total CN	P	100.5138	µg/l	5/3/2019 10:56:40	
250PPBCN	A	Total CN	P	249.8226	µg/l	5/3/2019 10:56:41	
500PPBCN	A	Total CN	P	500.0113	µg/l	5/3/2019 10:56:42	
ICV1	S	Total CN	P	95.7603	µg/l	5/3/2019 14:39:50	
ICB1	S	Total CN	P	0.5888	µg/l	5/3/2019 14:39:51	
CCV1	S	Total CN	P	244.6195	µg/l	5/3/2019 14:39:52	
CCB1	S	Total CN	P	0.3875	µg/l	5/3/2019 14:39:53	
PB119450BL	S	Total CN	P	0.4621	µg/l	5/3/2019 14:39:54	
PB119450BS	S	Total CN	P	98.935	µg/l	5/3/2019 14:39:55	
LOWPB119450	S	Total CN	P	10.215	µg/l	5/3/2019 14:39:56	
HIGHPB119450	S	Total CN	P	495.9057	µg/l	5/3/2019 14:39:57	
K2635-01	S	Total CN	P	1.8213	µg/l	5/3/2019 14:39:58	
K2635-01DUP	S	Total CN	P	1.5094	µg/l	5/3/2019 14:39:59	
K2635-01MS	S	Total CN	P	32.0471	µg/l	5/3/2019 14:40:00	
K2635-01MSD	S	Total CN	P	31.9932	µg/l	5/3/2019 14:47:25	
K2635-03	S	Total CN	P	1.2706	µg/l	5/3/2019 14:47:26	
K2635-05	S	Total CN	P	2.3417	µg/l	5/3/2019 14:47:27	
CCV2	S	Total CN	P	246.9566	µg/l	5/3/2019 14:47:28	
CCB2	S	Total CN	P	0.6907	µg/l	5/3/2019 14:47:29	
K2635-07	S	Total CN	P	1.2147	µg/l	5/3/2019 14:47:30	
K2642-01	S	Total CN	P	1.0938	µg/l	5/3/2019 14:47:31	
K2647-01	S	Total CN	P	3.0874	µg/l	5/3/2019 14:47:32	
K2647-03	S	Total CN	P	0.9046	µg/l	5/3/2019 14:47:33	
K2667-01	S	Total CN	P	2.5196	µg/l	5/3/2019 14:47:34	
K2667-03	S	Total CN	P	1.8921	µg/l	5/3/2019 14:47:35	
K2668-01	S	Total CN	P	0.4643	µg/l	5/3/2019 14:54:57	
K2668-03	S	Total CN	P	0.6818	µg/l	5/3/2019 14:54:58	
K2668-05	S	Total CN	P	0.7819	µg/l	5/3/2019 14:54:59	
K2677-01	S	Total CN	P	0.6835	µg/l	5/3/2019 14:55:00	
CCV3	S	Total CN	P	243.7956	µg/l	5/3/2019 14:55:01	
CCB3	S	Total CN	P	0.7712	µg/l	5/3/2019 14:55:02	
K2678-01	S	Total CN	P	3.7138	µg/l	5/3/2019 14:55:03	
K2678-01DUP	S	Total CN	P	3.5388	µg/l	5/3/2019 14:55:04	
K2678-01MS	S	Total CN	P	37.0568	µg/l	5/3/2019 14:55:05	
K2678-01MSD	S	Total CN	P	37.0937	µg/l	5/3/2019 14:55:06	
CCV4	S	Total CN	P	257.1875	µg/l	5/3/2019 15:00:15	
CCB4	S	Total CN	P	0.5356	µg/l	5/3/2019 15:00:16	