

LB102568

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/6/2019 14:29

Test: Reactive
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	99.068	0.0	0.102	
ICB1	0.095	0.0	0.005	
CCV1	247.161	0.0	0.248	
CCB1	-1.044	0.0	0.004	
PB119491BL	-0.355	0.0	0.004	
K2639-02	-0.750	0.0	0.004	
K2639-02DUP	-0.363	0.0	0.004	
K2639-04	-0.138	0.0	0.005	
K2672-02	-0.329	0.0	0.004	
K2672-04	-0.391	0.0	0.004	
K2672-08	-0.313	0.0	0.004	
K2672-10	-0.470	0.0	0.004	
K2672-06	-0.335	0.0	0.004	
K2672-12	0.043	0.0	0.005	
CCV2	245.963	0.0	0.247	
CCB2	0.207	0.0	0.005	
K2672-14	-0.348	0.0	0.004	
K2672-16	-0.295	0.0	0.004	
K2672-18	-0.428	0.0	0.004	
K2672-20	0.064	0.0	0.005	
K2680-01	-0.007	0.0	0.005	
K2680-02	-0.064	0.0	0.005	
K2680-03	-0.113	0.0	0.005	
K2689-01	-0.111	0.0	0.005	
K2703-01	0.081	0.0	0.005	
CCV3	264.268	0.0	0.265	
CCB3	-0.068	0.0	0.005	

N 27
Mean 31.520
SD 81.9046
CV% 259.85

Aquakem v. 7.2AQ1

Results from time period:

Mon May 06 12:20:35 2019

Mon May 06 14:20:26 2019

AS

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.6649	µg/l	5/6/2019 12:20:35	
5.OPPBCN	A	Reactive CN	P	4.2274	µg/l	5/6/2019 12:20:36	
10PPBCN	A	Reactive CN	P	9.6957	µg/l	5/6/2019 12:20:37	
50PPBCN	A	Reactive CN	P	50.6118	µg/l	5/6/2019 12:20:38	
100PPBCN	A	Reactive CN	P	100.9812	µg/l	5/6/2019 12:20:39	
250PPBCN	A	Reactive CN	P	250.7847	µg/l	5/6/2019 12:20:40	
500PPBCN	A	Reactive CN	P	499.3641	µg/l	5/6/2019 12:20:41	
ICV1	S	Reactive CN	P	99.0675	µg/l	5/6/2019 13:44:45	
ICB1	S	Reactive CN	P	0.0952	µg/l	5/6/2019 13:44:46	
CCV1	S	Reactive CN	P	247.1612	µg/l	5/6/2019 13:44:47	
CCB1	S	Reactive CN	P	-1.0442	µg/l	5/6/2019 13:44:48	
PB119491BL	S	Reactive CN	P	-0.3553	µg/l	5/6/2019 13:44:49	
K2639-02	S	Reactive CN	P	-0.75	µg/l	5/6/2019 13:44:50	
K2639-02DUP	S	Reactive CN	P	-0.363	µg/l	5/6/2019 13:44:51	
K2639-04	S	Reactive CN	P	-0.1378	µg/l	5/6/2019 13:44:52	
K2672-02	S	Reactive CN	P	-0.3295	µg/l	5/6/2019 13:44:53	
K2672-04	S	Reactive CN	P	-0.3909	µg/l	5/6/2019 13:44:54	
K2672-08	S	Reactive CN	P	-0.3131	µg/l	5/6/2019 13:44:55	
K2672-10	S	Reactive CN	P	-0.4696	µg/l	5/6/2019 13:52:17	
K2672-06	S	Reactive CN	P	-0.3345	µg/l	5/6/2019 13:52:18	
K2672-12	S	Reactive CN	P	0.0433	µg/l	5/6/2019 13:52:19	
CCV2	S	Reactive CN	P	245.9627	µg/l	5/6/2019 14:16:33	
CCB2	S	Reactive CN	P	0.2071	µg/l	5/6/2019 14:16:34	
K2672-14	S	Reactive CN	P	-0.3482	µg/l	5/6/2019 14:16:35	
K2672-16	S	Reactive CN	P	-0.2955	µg/l	5/6/2019 14:16:36	
K2672-18	S	Reactive CN	P	-0.4277	µg/l	5/6/2019 14:16:37	
K2672-20	S	Reactive CN	P	0.064	µg/l	5/6/2019 14:16:38	
K2680-01	S	Reactive CN	P	-0.0072	µg/l	5/6/2019 14:16:39	
K2680-02	S	Reactive CN	P	-0.0638	µg/l	5/6/2019 14:16:40	
K2680-03	S	Reactive CN	P	-0.1132	µg/l	5/6/2019 14:16:41	
K2689-01	S	Reactive CN	P	-0.1107	µg/l	5/6/2019 14:16:42	
K2703-01	S	Reactive CN	P	0.0806	µg/l	5/6/2019 14:16:43	
CCV3	S	Reactive CN	P	264.2684	µg/l	5/6/2019 14:20:25	
CCB3	S	Reactive CN	P	-0.0676	µg/l	5/6/2019 14:20:26	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/6/2019 12:23


Test Total CN

Accepted 5/6/2019 12:23

Factor 1017
Bias 0.005

Coeff. of det. 0.999983

Errors

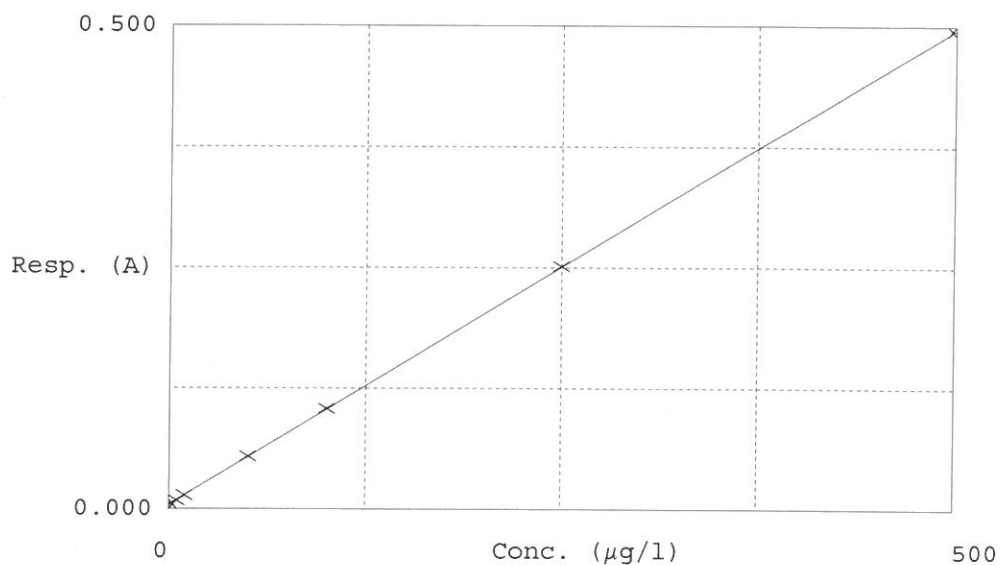

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.6649	0.0000	
2	5.0PPBCN	0.009	4.2274	5.0000	
3	10PPBCN	0.014	9.6957	10.0000	
4	50PPBCN	0.054	50.6118	50.0000	
5	100PPBCN	0.104	100.9812	100.0000	
6	250PPBCN	0.251	250.7847	250.0000	
7	500PPBCN	0.496	499.3641	500.0000	