

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AS

Instrument ID : Konelab

5/7/2019 14:57

Test: *Reactive*
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.639	0.0	0.102	
ICB1	-0.805	0.0	0.005	
CCV1	240.829	0.0	0.245	
CCB1	-1.016	0.0	0.004	
PB119515BL	-0.904	0.0	0.005	
K2673-02	-1.062	0.0	0.004	
K2673-02DUP	-1.224	0.0	0.004	
K2673-04	-1.272	0.0	0.004	
K2673-06	-1.155	0.0	0.004	
K2673-08	-1.237	0.0	0.004	
K2673-10	-1.255	0.0	0.004	
K2673-12	-1.319	0.0	0.004	
K2673-14	-1.199	0.0	0.004	
K2673-15	-0.930	0.0	0.005	
CCV2	241.895	0.0	0.246	
CCB2	-0.964	0.0	0.005	
K2673-16	-1.111	0.0	0.004	
K2698-02	-1.274	0.0	0.004	
PB119516BL	-1.124	0.0	0.004	
K2696-02	-1.134	0.0	0.004	
K2696-02DUP	-1.281	0.0	0.004	
CCV3	258.100	0.0	0.262	
CCB3	-0.916	0.0	0.005	

N	23
Mean	35.490
SD	86.2134
CV%	242.92

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/7/2019 14:18


Test Total CN

Accepted 5/7/2019 14:18

Factor 1006
Bias 0.005

Coeff. of det. 0.999920

Errors

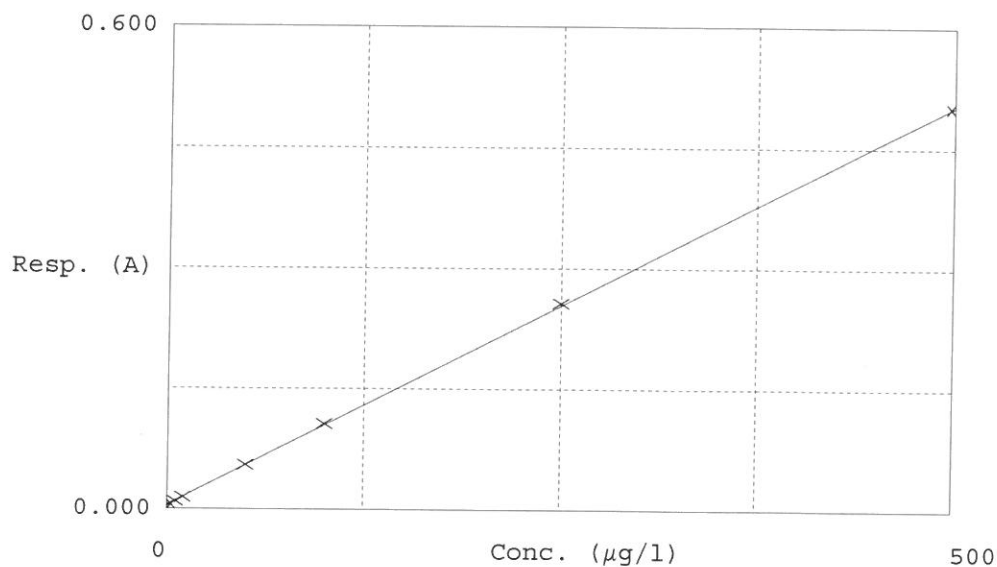

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-1.1114	0.0000	
2	5.0PPBCN	0.010	4.2236	5.0000	
3	10PPBCN	0.015	9.2722	10.0000	
4	50PPBCN	0.055	49.9773	50.0000	
5	100PPBCN	0.106	101.3915	100.0000	
6	250PPBCN	0.257	253.0011	250.0000	
7	500PPBCN	0.501	498.2458	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Tue May 07 14:17:42 2019

Tue May 07 14:56:28 2019

AS

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-1.1114	µg/l	5/7/2019 14:17:42	
5.OPPBCN	A	Reactive CN	P	4.2236	µg/l	5/7/2019 14:17:43	
10PPBCN	A	Reactive CN	P	9.2722	µg/l	5/7/2019 14:17:44	
50PPBCN	A	Reactive CN	P	49.9773	µg/l	5/7/2019 14:17:45	
100PPBCN	A	Reactive CN	P	101.3915	µg/l	5/7/2019 14:17:46	
250PPBCN	A	Reactive CN	P	253.0011	µg/l	5/7/2019 14:17:47	
500PPBCN	A	Reactive CN	P	498.2458	µg/l	5/7/2019 14:17:48	
ICV1	S	Reactive CN	P	96.6386	µg/l	5/7/2019 14:45:29	
ICB1	S	Reactive CN	P	-0.8051	µg/l	5/7/2019 14:45:30	
CCV1	S	Reactive CN	P	240.829	µg/l	5/7/2019 14:45:31	
CCB1	S	Reactive CN	P	-1.0156	µg/l	5/7/2019 14:45:32	
PB119515BL	S	Reactive CN	P	-0.9044	µg/l	5/7/2019 14:45:33	
K2673-02	S	Reactive CN	P	-1.0616	µg/l	5/7/2019 14:45:34	
K2673-02DUP	S	Reactive CN	P	-1.2242	µg/l	5/7/2019 14:45:35	
K2673-04	S	Reactive CN	P	-1.2724	µg/l	5/7/2019 14:45:36	
K2673-06	S	Reactive CN	P	-1.1555	µg/l	5/7/2019 14:45:37	
K2673-08	S	Reactive CN	P	-1.2374	µg/l	5/7/2019 14:45:38	
K2673-10	S	Reactive CN	P	-1.2554	µg/l	5/7/2019 14:45:39	
K2673-12	S	Reactive CN	P	-1.3192	µg/l	5/7/2019 14:53:04	
K2673-14	S	Reactive CN	P	-1.1986	µg/l	5/7/2019 14:53:05	
K2673-15	S	Reactive CN	P	-0.9303	µg/l	5/7/2019 14:53:06	
CCV2	S	Reactive CN	P	241.8953	µg/l	5/7/2019 14:53:07	
CCB2	S	Reactive CN	P	-0.9639	µg/l	5/7/2019 14:53:08	
K2673-16	S	Reactive CN	P	-1.1115	µg/l	5/7/2019 14:53:09	
K2698-02	S	Reactive CN	P	-1.2742	µg/l	5/7/2019 14:53:10	
PB119516BL	S	Reactive CN	P	-1.1241	µg/l	5/7/2019 14:53:12	
K2696-02	S	Reactive CN	P	-1.1343	µg/l	5/7/2019 14:53:13	
K2696-02DUP	S	Reactive CN	P	-1.2808	µg/l	5/7/2019 14:53:14	
CCV3	S	Reactive CN	P	258.1002	µg/l	5/7/2019 14:56:27	
CCB3	S	Reactive CN	P	-0.9158	µg/l	5/7/2019 14:56:28	