

213162635

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/9/2019 12:19

Test: *Reaction*
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.533	0.0	0.105	
ICB1	-0.223	0.0	0.004	
CCV1	244.605	0.0	0.256	
CCB1	-0.344	0.0	0.004	
PB119581BL	-0.491	0.0	0.004	
K2746-02	-0.026	0.0	0.004	
K2746-02DUP	-0.694	0.0	0.004	
K2750-01	-0.546	0.0	0.004	
K2750-05	-0.546	0.0	0.004	
K2754-06	-0.723	0.0	0.004	
K2754-08	-0.340	0.0	0.004	
CCV2	257.036	0.0	0.268	
CCB2	-0.438	0.0	0.004	

N	13
Mean	45.754
SD	94.9558
CV%	207.54

AS

Aquakem v. 7.2AQ1

Results from time period:

Thu May 09 09:44:07 2019

Thu May 09 12:18:44 2019

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.7791	µg/l	5/9/2019 9:44:07	
5.OPPBCN	A	Reactive CN	P	4.5273	µg/l	5/9/2019 9:44:08	
10PPBCN	A	Reactive CN	P	9.4311	µg/l	5/9/2019 9:44:09	
50PPBCN	A	Reactive CN	P	48.9539	µg/l	5/9/2019 9:44:10	
100PPBCN	A	Reactive CN	P	100.9932	µg/l	5/9/2019 9:44:11	
250PPBCN	A	Reactive CN	P	253.9032	µg/l	5/9/2019 9:44:12	
500PPBCN	A	Reactive CN	P	497.9705	µg/l	5/9/2019 9:44:13	
ICV1	S	Reactive CN	P	97.5326	µg/l	5/9/2019 12:15:20	
ICB1	S	Reactive CN	P	-0.2232	µg/l	5/9/2019 12:15:21	
CCV1	S	Reactive CN	P	244.6047	µg/l	5/9/2019 12:15:22	
CCB1	S	Reactive CN	P	-0.3439	µg/l	5/9/2019 12:15:23	
PB119581BL	S	Reactive CN	P	-0.4913	µg/l	5/9/2019 12:15:24	
K2746-02	S	Reactive CN	P	-0.0263	µg/l	5/9/2019 12:15:25	
K2746-02DUP	S	Reactive CN	P	-0.6939	µg/l	5/9/2019 12:15:26	
K2750-01	S	Reactive CN	P	-0.5457	µg/l	5/9/2019 12:15:27	
K2750-05	S	Reactive CN	P	-0.5458	µg/l	5/9/2019 12:15:28	
K2754-06	S	Reactive CN	P	-0.7227	µg/l	5/9/2019 12:15:29	
K2754-08	S	Reactive CN	P	-0.3395	µg/l	5/9/2019 12:15:30	
CCV2	S	Reactive CN	P	257.036	µg/l	5/9/2019 12:18:43	
CCB2	S	Reactive CN	P	-0.4384	µg/l	5/9/2019 12:18:44	

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/9/2019 9:47

Test Total CN


Accepted 5/9/2019 9:47

Factor 973.9

Bias 0.005

Coeff. of det. 0.999890

Errors

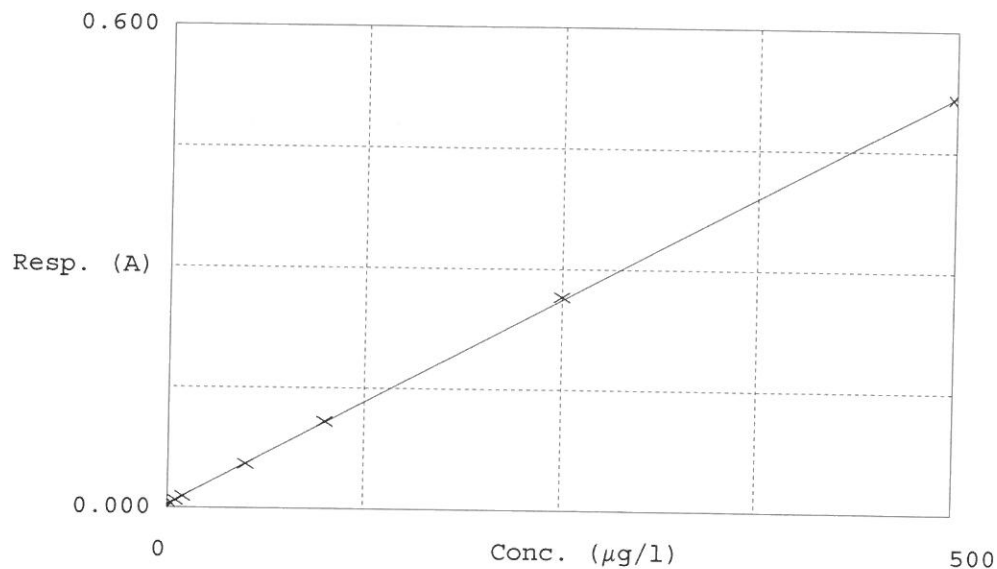

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.7791	0.0000	
2	5.0PPBCN	0.009	4.5273	5.0000	
3	10PPBCN	0.014	9.4311	10.0000	
4	50PPBCN	0.055	48.9539	50.0000	
5	100PPBCN	0.108	100.9932	100.0000	
6	250PPBCN	0.265	253.9032	250.0000	
7	500PPBCN	0.516	497.9705	500.0000	