

2/102980

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/24/2019 11:25

Test: Reactive
Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.751	0.0	0.102	
ICB1	0.774	0.0	0.004	
CCV1	236.965	0.0	0.247	
CCB1	0.649	0.0	0.004	
PB120037BL	0.410	0.0	0.004	
K2643-10	0.617	0.0	0.004	
K2643-10DUP	0.556	0.0	0.004	
K2643-12	0.496	0.0	0.004	
K3019-03	0.711	0.0	0.004	
K3019-06	0.546	0.0	0.004	
K3019-09	0.071	0.0	0.004	
K3023-01	0.525	0.0	0.004	
K3026-04	0.597	0.0	0.004	
K3026-08	0.658	0.0	0.004	
CCV2	238.463	0.0	0.248	
CCB2	0.560	0.0	0.004	
K3026-16	0.577	0.0	0.004	
K3035-01	0.417	0.0	0.004	
CCV3	241.716	0.0	0.251	
CCB3	0.953	0.0	0.005	

N	20
Mean	41.101
SD	87.9091
CV%	213.89

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/24/2019 10:42


Test Total CN

Accepted 5/24/2019 10:42

Factor 975.2
Bias 0.004

Coeff. of det. 0.999888

Errors

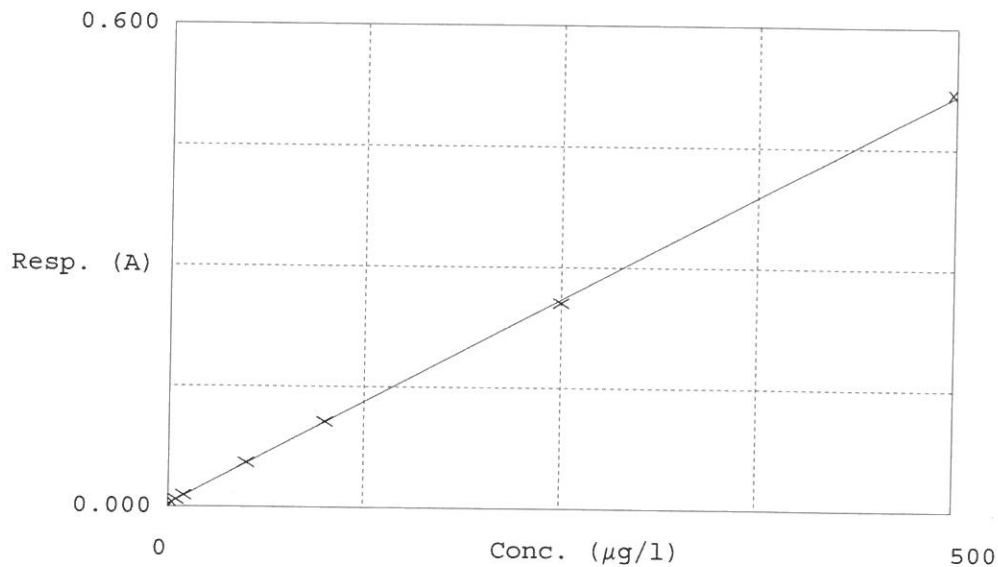

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.4736	0.0000	
2	5.0PPBCN	0.009	5.3182	5.0000	
3	10PPBCN	0.014	10.6601	10.0000	
4	50PPBCN	0.055	50.5291	50.0000	
5	100PPBCN	0.106	100.2561	100.0000	
6	250PPBCN	0.256	245.7668	250.0000	
7	500PPBCN	0.518	501.9961	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri May 24 10:40:21 2019

Fri May 24 11:21:14 2019

AS

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.4736	µg/l	5/24/2019 10:40:21	
5.OPPBCN	A	Reactive CN	P	5.3182	µg/l	5/24/2019 10:40:22	
10PPBCN	A	Reactive CN	P	10.6601	µg/l	5/24/2019 10:40:23	
50PPBCN	A	Reactive CN	P	50.5291	µg/l	5/24/2019 10:40:24	
100PPBCN	A	Reactive CN	P	100.2561	µg/l	5/24/2019 10:40:25	
250PPBCN	A	Reactive CN	P	245.7668	µg/l	5/24/2019 10:40:26	
500PPBCN	A	Reactive CN	P	501.9961	µg/l	5/24/2019 10:40:27	
ICV1	S	Reactive CN	P	95.7509	µg/l	5/24/2019 11:13:58	
ICB1	S	Reactive CN	P	0.7738	µg/l	5/24/2019 11:13:59	
CCV1	S	Reactive CN	P	236.9648	µg/l	5/24/2019 11:14:00	
CCB1	S	Reactive CN	P	0.6491	µg/l	5/24/2019 11:14:01	
PB120037BL	S	Reactive CN	P	0.4103	µg/l	5/24/2019 11:14:02	
K2643-10	S	Reactive CN	P	0.6168	µg/l	5/24/2019 11:14:03	
K2643-10DUP	S	Reactive CN	P	0.5555	µg/l	5/24/2019 11:14:04	
K2643-12	S	Reactive CN	P	0.4963	µg/l	5/24/2019 11:14:05	
K3019-03	S	Reactive CN	P	0.7108	µg/l	5/24/2019 11:14:06	
K3019-06	S	Reactive CN	P	0.546	µg/l	5/24/2019 11:14:07	
K3019-09	S	Reactive CN	P	0.0706	µg/l	5/24/2019 11:14:08	
K3023-01	S	Reactive CN	P	0.5251	µg/l	5/24/2019 11:21:05	
K3026-04	S	Reactive CN	P	0.5966	µg/l	5/24/2019 11:21:06	
K3026-08	S	Reactive CN	P	0.6581	µg/l	5/24/2019 11:21:07	
CCV2	S	Reactive CN	P	238.4629	µg/l	5/24/2019 11:21:08	
CCB2	S	Reactive CN	P	0.5598	µg/l	5/24/2019 11:21:09	
K3026-16	S	Reactive CN	P	0.5773	µg/l	5/24/2019 11:21:10	
K3035-01	S	Reactive CN	P	0.4167	µg/l	5/24/2019 11:21:11	
CCV3	S	Reactive CN	P	241.7156	µg/l	5/24/2019 11:21:13	
CCB3	S	Reactive CN	P	0.9533	µg/l	5/24/2019 11:21:14	