

2B103095

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/30/2019 14:01

Test: Total CN

Mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.690	0.0	0.100	
ICB1	0.017	0.0	0.004	
CCV1	237.654	0.0	0.242	
CCB1	0.242	0.0	0.004	
PB120185BL	-0.215	0.0	0.004	
K2642-08	-0.028	0.0	0.004	
K2642-08DUP	-0.252	0.0	0.004	
K2648-04	-0.263	0.0	0.004	
K3090-04	-0.102	0.0	0.004	
K3090-10	-0.071	0.0	0.004	
PB120186BL	-0.389	0.0	0.003	
K3085-02	-0.282	0.0	0.004	
K3085-02DUP	-0.013	0.0	0.004	
CCV2	251.571	0.0	0.256	
CCB2	0.067	0.0	0.004	

N	15
Mean	38.908
SD	87.1027
CV%	223.87

Aquakem v. 7.2AQ1

Results from time period:

Thu May 30 13:56:07 2019

Thu May 30 14:00:58 2019

A

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.3457	µg/l	5/30/2019 10:59:35	
5.0PPBCN	A	Reactive CN	P	5.1797	µg/l	5/30/2019 10:59:36	
10PPBCN	A	Reactive CN	P	9.1993	µg/l	5/30/2019 10:59:37	
50PPBCN	A	Reactive CN	P	49.3119	µg/l	5/30/2019 10:59:38	
100PPBCN	A	Reactive CN	P	100.7169	µg/l	5/30/2019 10:59:39	
250PPBCN	A	Reactive CN	P	251.9966	µg/l	5/30/2019 10:59:40	
500PPBCN	A	Reactive CN	P	498.9414	µg/l	5/30/2019 10:59:41	
ICV1	S	Reactive CN	P	95.6902	µg/l	5/30/2019 13:56:07	
ICB1	S	Reactive CN	P	0.0168	µg/l	5/30/2019 13:56:08	
CCV1	S	Reactive CN	P	237.6536	µg/l	5/30/2019 13:56:09	
CCB1	S	Reactive CN	P	0.242	µg/l	5/30/2019 13:56:10	
PB120185BL	S	Reactive CN	P	-0.2147	µg/l	5/30/2019 13:56:11	
K2642-08	S	Reactive CN	P	-0.0283	µg/l	5/30/2019 13:56:12	
K2642-08DUP	S	Reactive CN	P	-0.2525	µg/l	5/30/2019 13:56:13	
K2648-04	S	Reactive CN	P	-0.2627	µg/l	5/30/2019 13:56:14	
K3090-04	S	Reactive CN	P	-0.1015	µg/l	5/30/2019 13:56:15	
K3090-10	S	Reactive CN	P	-0.071	µg/l	5/30/2019 13:56:16	
PB120186BL	S	Reactive CN	P	-0.3888	µg/l	5/30/2019 13:56:17	
K3085-02	S	Reactive CN	P	-0.2821	µg/l	5/30/2019 14:00:54	
K3085-02DUP	S	Reactive CN	P	-0.0128	µg/l	5/30/2019 14:00:55	
CCV2	S	Reactive CN	P	251.5707	µg/l	5/30/2019 14:00:57	
CCB2	S	Reactive CN	P	0.0669	µg/l	5/30/2019 14:00:58	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/30/2019 11:12


Test Total CN

Accepted 5/30/2019 11:12

Factor 998.1
Bias 0.004

Coeff. of det. 0.999967

Errors

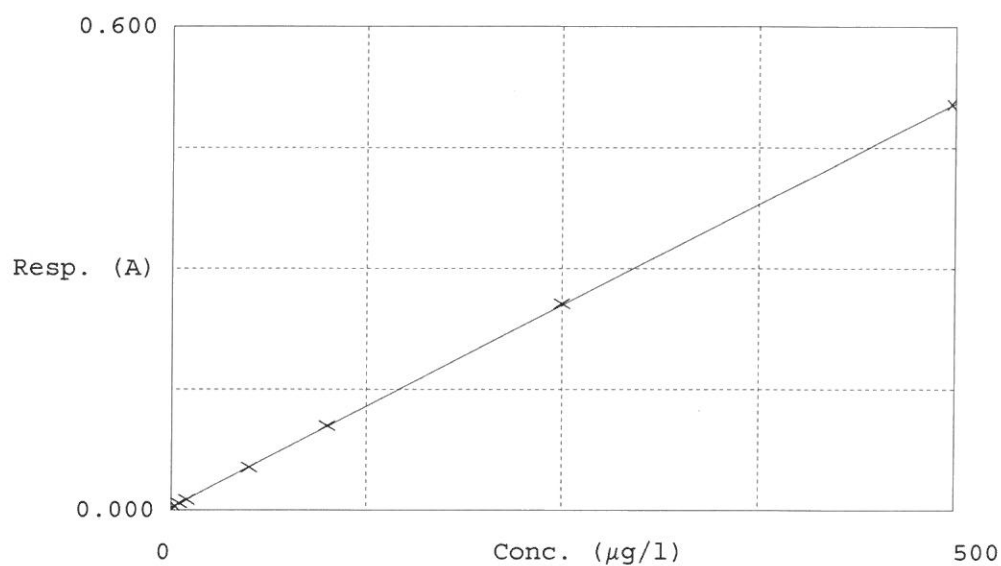

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.3457	0.0000	
2	5.0PPBCN	0.009	5.1797	5.0000	
3	10PPBCN	0.013	9.1993	10.0000	
4	50PPBCN	0.053	49.3119	50.0000	
5	100PPBCN	0.105	100.7169	100.0000	
6	250PPBCN	0.256	251.9966	250.0000	
7	500PPBCN	0.504	498.9414	500.0000	