

=====

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AS

Instrument ID : Konelab

6/3/2019 13:22

Test: Total CN

Mg/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.183	0.0	0.099	
ICB1	0.297	0.0	0.004	
CCV1	238.288	0.0	0.236	
CCB1	-0.068	0.0	0.004	
PB120281BL	-0.068	0.0	0.004	
PB120281BS	97.645	0.0	0.099	
LOWPB120281	9.789	0.0	0.013	
HIGHPB120281	483.209	0.0	0.475	
K2641-13	1.327	0.0	0.005	
K2641-13DUP	0.976	0.0	0.005	
K2641-13MS	39.747	0.0	0.042	
K2641-13MSD	39.650	0.0	0.042	
K2641-15	1.342	0.0	0.005	
K2641-17	0.554	0.0	0.004	
CCV2	239.786	0.0	0.238	
CCB2	0.091	0.0	0.004	
K2641-19	-0.019	0.0	0.004	
K2641-21	0.978	0.0	0.005	
K3135-01	0.181	0.0	0.004	
K3139-03	-0.149	0.0	0.003	
K3139-07	-0.225	0.0	0.003	
CCV3	251.456	0.0	0.249	
CCB3	0.118	0.0	0.004	

N	23
Mean	65.308
SD	123.4235
CV%	188.99

Aquakem v. 7.2AQ1

Results from time period:

Mon Jun 03 11:48:35 2019

Mon Jun 03 13:15:41 2019

✓ AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.2019	µg/l	6/3/2019 11:48:35	
5.0PPBCN	A	Total CN	P	4.3799	µg/l	6/3/2019 11:48:36	
10PPBCN	A	Total CN	P	9.6099	µg/l	6/3/2019 11:48:37	
50PPBCN	A	Total CN	P	49.9935	µg/l	6/3/2019 11:48:38	
100PPBCN	A	Total CN	P	101.2708	µg/l	6/3/2019 11:48:39	
250PPBCN	A	Total CN	P	250.3746	µg/l	6/3/2019 11:48:40	
500PPBCN	A	Total CN	P	499.5732	µg/l	6/3/2019 11:48:41	
ICV1	S	Total CN	P	97.1832	µg/l	6/3/2019 13:03:46	
ICB1	S	Total CN	P	0.297	µg/l	6/3/2019 13:03:47	
CCV1	S	Total CN	P	238.2878	µg/l	6/3/2019 13:03:48	
CCB1	S	Total CN	P	-0.0677	µg/l	6/3/2019 13:03:49	
PB120281BL	S	Total CN	P	-0.0676	µg/l	6/3/2019 13:03:50	
PB120281BS	S	Total CN	P	97.6446	µg/l	6/3/2019 13:03:51	
LOWPB120281	S	Total CN	P	9.7885	µg/l	6/3/2019 13:03:52	
HIGHPB120281	S	Total CN	P	483.209	µg/l	6/3/2019 13:03:53	
K2641-13	S	Total CN	P	1.3272	µg/l	6/3/2019 13:03:54	
K2641-13DUP	S	Total CN	P	0.9763	µg/l	6/3/2019 13:03:55	
K2641-13MS	S	Total CN	P	39.7465	µg/l	6/3/2019 13:03:56	
K2641-13MSD	S	Total CN	P	39.6495	µg/l	6/3/2019 13:11:19	
K2641-15	S	Total CN	P	1.3417	µg/l	6/3/2019 13:11:20	
K2641-17	S	Total CN	P	0.5542	µg/l	6/3/2019 13:11:21	
CCV2	S	Total CN	P	239.7862	µg/l	6/3/2019 13:11:22	
CCB2	S	Total CN	P	0.0908	µg/l	6/3/2019 13:11:23	
K2641-19	S	Total CN	P	-0.0192	µg/l	6/3/2019 13:11:24	
K2641-21	S	Total CN	P	0.9779	µg/l	6/3/2019 13:11:25	
K3135-01	S	Total CN	P	0.1805	µg/l	6/3/2019 13:11:26	
K3139-03	S	Total CN	P	-0.1486	µg/l	6/3/2019 13:11:27	
K3139-07	S	Total CN	P	-0.2254	µg/l	6/3/2019 13:11:28	
CCV3	S	Total CN	P	251.4564	µg/l	6/3/2019 13:15:39	
CCB3	S	Total CN	P	0.118	µg/l	6/3/2019 13:15:40	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

Instrument ID : Konelab

6/3/2019 12:31


Test Total CN

Accepted 6/3/2019 12:31

Factor 1024
 Bias 0.004

Coeff. of det. 0.999988

Errors

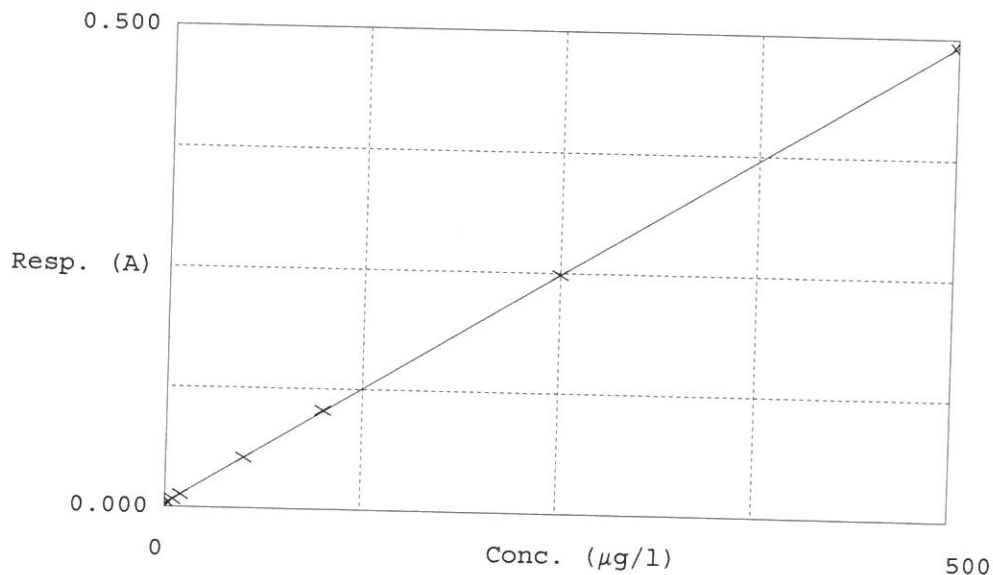

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.2019	0.0000	
2	5.0PPBCN	0.008	4.3799	5.0000	
3	10PPBCN	0.013	9.6099	10.0000	
4	50PPBCN	0.052	49.9935	50.0000	
5	100PPBCN	0.103	101.2708	100.0000	
6	250PPBCN	0.248	250.3746	250.0000	
7	500PPBCN	0.491	499.5732	500.0000	