

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/6/2019 13:02

Test: Total CN

Sample Id	<i>Mg/d</i> Result	Dil. 1 +	Response	Errors
ICV1	96.895	0.0	0.101	
ICB1	1.269	0.0	0.005	
CCV1	243.179	0.0	0.249	
CCB1	0.270	0.0	0.004	
PB120390BL	1.239	0.0	0.005	
K3153-02	0.616	0.0	0.004	
K3153-02DUP	0.132	0.0	0.004	
K3153-04	0.352	0.0	0.004	
K3153-06	0.402	0.0	0.004	
K3192-02	-0.126	0.0	0.004	
K3211-02	-0.028	0.0	0.004	
K3211-04	0.257	0.0	0.004	
K3211-06	0.296	0.0	0.004	
K3211-08	0.368	0.0	0.004	
CCV2	241.670	0.0	0.247	
CCB2	0.473	0.0	0.004	
K3218-03	0.229	0.0	0.004	
K3218-06	-0.290	0.0	0.004	
K3218-09	-0.027	0.0	0.004	
K3156-02	-0.025	0.0	0.004	
CCV3	243.917	0.0	0.250	
CCB3	0.058	0.0	0.004	

N	22
Mean	37.778
SD	85.9209
CV%	227.43

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

Instrument ID : Konelab

6/6/2019 11:37


Test Total CN

Accepted 6/6/2019 11:37

Factor 992.1
 Bias 0.004

Coeff. of det. 0.999994

Errors

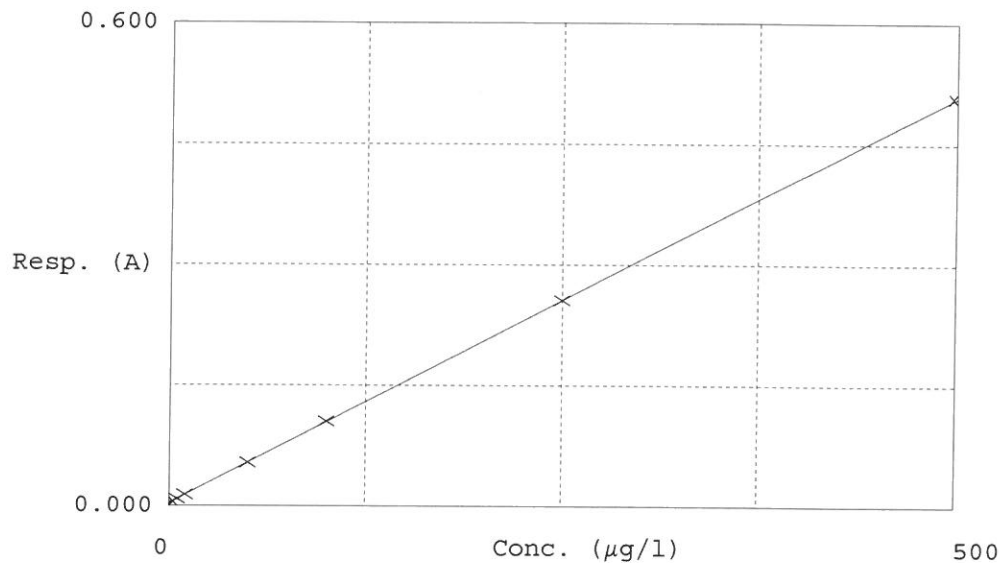

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.1610	0.0000	
2	5.0PPBCN	0.008	4.5965	5.0000	
3	10PPBCN	0.014	9.9935	10.0000	
4	50PPBCN	0.054	49.6992	50.0000	
5	100PPBCN	0.106	100.9086	100.0000	
6	250PPBCN	0.256	250.2212	250.0000	
7	500PPBCN	0.508	499.7419	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Thu Jun 06 11:34:56 2019

Thu Jun 06 12:50:57 2019

AS

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.161	µg/l	6/6/2019 11:34:56	
5.OPPBCN	A	Reactive CN	P	4.5965	µg/l	6/6/2019 11:34:57	
10PPBCN	A	Reactive CN	P	9.9935	µg/l	6/6/2019 11:34:58	
50PPBCN	A	Reactive CN	P	49.6992	µg/l	6/6/2019 11:34:59	
100PPBCN	A	Reactive CN	P	100.9086	µg/l	6/6/2019 11:35:00	
250PPBCN	A	Reactive CN	P	250.2212	µg/l	6/6/2019 11:35:01	
500PPBCN	A	Reactive CN	P	499.7419	µg/l	6/6/2019 11:35:02	
ICV1	S	Reactive CN	P	96.895	µg/l	6/6/2019 12:43:12	
ICB1	S	Reactive CN	P	1.2688	µg/l	6/6/2019 12:43:13	
CCV1	S	Reactive CN	P	243.179	µg/l	6/6/2019 12:43:14	
CCB1	S	Reactive CN	P	0.27	µg/l	6/6/2019 12:43:15	
PB120390BL	S	Reactive CN	P	1.2395	µg/l	6/6/2019 12:43:16	
K3153-02	S	Reactive CN	P	0.6164	µg/l	6/6/2019 12:43:17	
K3153-02DUP	S	Reactive CN	P	0.1316	µg/l	6/6/2019 12:43:18	
K3153-04	S	Reactive CN	P	0.3522	µg/l	6/6/2019 12:43:19	
K3153-06	S	Reactive CN	P	0.4018	µg/l	6/6/2019 12:43:20	
K3192-02	S	Reactive CN	P	-0.1256	µg/l	6/6/2019 12:43:21	
K3211-02	S	Reactive CN	P	-0.0279	µg/l	6/6/2019 12:43:22	
K3211-04	S	Reactive CN	P	0.2567	µg/l	6/6/2019 12:50:47	
K3211-06	S	Reactive CN	P	0.2957	µg/l	6/6/2019 12:50:48	
K3211-08	S	Reactive CN	P	0.3684	µg/l	6/6/2019 12:50:49	
CCV2	S	Reactive CN	P	241.67	µg/l	6/6/2019 12:50:50	
CCB2	S	Reactive CN	P	0.4726	µg/l	6/6/2019 12:50:51	
K3218-03	S	Reactive CN	P	0.2287	µg/l	6/6/2019 12:50:52	
K3218-06	S	Reactive CN	P	-0.2904	µg/l	6/6/2019 12:50:53	
K3218-09	S	Reactive CN	P	-0.0271	µg/l	6/6/2019 12:50:54	
K3156-02	S	Reactive CN	P	-0.0246	µg/l	6/6/2019 12:50:55	
CCV3	S	Reactive CN	P	243.9168	µg/l	6/6/2019 12:50:56	
CCB3	S	Reactive CN	P	0.0578	µg/l	6/6/2019 12:50:57	