

213103271

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/7/2019 14:08

Test: ~~Total~~ ^{Reactive} CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.556	0.0	0.107	
ICB1	0.397	0.0	0.004	
CCV1	242.493	0.0	0.260	
CCB1	0.135	0.0	0.004	
PB120432BL	0.309	0.0	0.004	
K3236-02	0.433	0.0	0.004	
K3236-02DUP	0.043	0.0	0.004	
PB120429BL	-0.284	0.0	0.004	
K3158-02	-0.534	0.0	0.003	
K3158-02DUP	-0.426	0.0	0.003	
K3160-02	-0.571	0.0	0.003	
K3160-04	-0.060	0.0	0.004	
CCV2	244.372	0.0	0.262	
CCB2	-0.265	0.0	0.004	
K3160-06	-0.094	0.0	0.004	
K3250-01	-0.196	0.0	0.004	
K3250-02	-0.119	0.0	0.004	
CCV3	248.369	0.0	0.266	
CCB3	-0.037	0.0	0.004	

N	19
Mean	43.764
SD	92.2964
CV%	210.89

AS

Aquakem v. 7.2AQ1

Results from time period:

Fri Jun 07 11:18:50 2019

Fri Jun 07 14:01:57 2019

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.1887	µg/l	6/7/2019 11:18:50	
5.0PPBCN	A	Reactive CN	P	4.3621	µg/l	6/7/2019 11:18:51	
10PPBCN	A	Reactive CN	P	9.7394	µg/l	6/7/2019 11:18:52	
50PPBCN	A	Reactive CN	P	49.9264	µg/l	6/7/2019 11:18:53	
100PPBCN	A	Reactive CN	P	100.5791	µg/l	6/7/2019 11:18:54	
250PPBCN	A	Reactive CN	P	251.357	µg/l	6/7/2019 11:18:55	
500PPBCN	A	Reactive CN	P	499.2247	µg/l	6/7/2019 11:18:56	
ICV1	S	Reactive CN	P	97.5563	µg/l	6/7/2019 13:55:39	
ICB1	S	Reactive CN	P	0.3965	µg/l	6/7/2019 13:55:40	
CCV1	S	Reactive CN	P	242.4929	µg/l	6/7/2019 13:55:41	
CCB1	S	Reactive CN	P	0.1346	µg/l	6/7/2019 13:55:42	
PB120432BL	S	Reactive CN	P	0.3091	µg/l	6/7/2019 13:55:43	
K3236-02	S	Reactive CN	P	0.4328	µg/l	6/7/2019 13:55:44	
K3236-02DUP	S	Reactive CN	P	0.0428	µg/l	6/7/2019 13:55:45	
PB120429BL	S	Reactive CN	P	-0.2839	µg/l	6/7/2019 13:55:46	
K3158-02	S	Reactive CN	P	-0.5337	µg/l	6/7/2019 13:55:47	
K3158-02DUP	S	Reactive CN	P	-0.4259	µg/l	6/7/2019 13:55:48	
K3160-02	S	Reactive CN	P	-0.5711	µg/l	6/7/2019 13:55:49	
K3160-04	S	Reactive CN	P	-0.0598	µg/l	6/7/2019 14:01:50	
CCV2	S	Reactive CN	P	244.3717	µg/l	6/7/2019 14:01:51	
CCB2	S	Reactive CN	P	-0.2651	µg/l	6/7/2019 14:01:52	
K3160-06	S	Reactive CN	P	-0.0943	µg/l	6/7/2019 14:01:53	
K3250-01	S	Reactive CN	P	-0.1955	µg/l	6/7/2019 14:01:54	
K3250-02	S	Reactive CN	P	-0.1195	µg/l	6/7/2019 14:01:55	
CCV3	S	Reactive CN	P	248.3685	µg/l	6/7/2019 14:01:56	
CCB3	S	Reactive CN	P	-0.0365	µg/l	6/7/2019 14:01:57	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/7/2019 11:22


Test Total CN

Accepted 6/7/2019 11:22

Factor 947.8
Bias 0.004

Coeff. of det. 0.999984

Errors

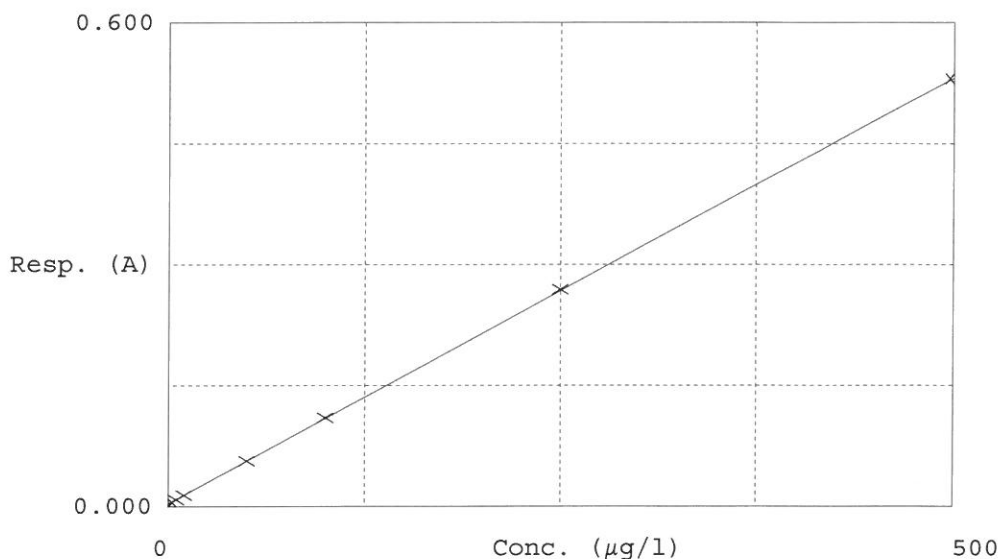

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.1887	0.0000	
2	5.0PPBCN	0.008	4.3621	5.0000	
3	10PPBCN	0.014	9.7394	10.0000	
4	50PPBCN	0.057	49.9264	50.0000	
5	100PPBCN	0.110	100.5791	100.0000	
6	250PPBCN	0.269	251.3570	250.0000	
7	500PPBCN	0.531	499.2247	500.0000	