

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/10/2019 14:16

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.007	0.0	0.102	
ICB1	0.334	0.0	0.004	
CCV1	240.893	0.0	0.247	
CCB1	0.301	0.0	0.004	
PB120480BL	0.124	0.0	0.004	
K3163-06	0.166	0.0	0.004	
K3163-06DUP	0.093	0.0	0.004	
K3163-08	0.048	0.0	0.004	
K3265-09	-0.136	0.0	0.004	
K3265-10	-0.043	0.0	0.004	
K3265-11	-0.210	0.0	0.003	
K3265-12	-0.645	0.0	0.003	
K3262-01	-0.132	0.0	0.004	
CCV2	254.435	0.0	0.261	
CCB2	0.089	0.0	0.004	

N	15
Mean	39.488
SD	88.1508
CV%	223.23

2B103312

Aquakem v. 7.2AQ1

Results from time period:

Mon Jun 10 14:11:03 2019

Mon Jun 10 14:15:54 2019

Sample Id	Sam/Ctr/c/	Test short	nan	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive	CN	P	-0.1135	µg/l	6/10/2019 11:30:44	
5.0PPBCN	A	Reactive	CN	P	4.8579	µg/l	6/10/2019 11:30:45	
10PPBCN	A	Reactive	CN	P	9.8534	µg/l	6/10/2019 11:30:46	
50PPBCN	A	Reactive	CN	P	49.3451	µg/l	6/10/2019 11:30:47	
100PPBCN	A	Reactive	CN	P	100.5933	µg/l	6/10/2019 11:30:48	
250PPBCN	A	Reactive	CN	P	251.0253	µg/l	6/10/2019 11:30:49	
500PPBCN	A	Reactive	CN	P	499.4385	µg/l	6/10/2019 11:30:50	
ICV1	S	Reactive	CN	P	97.0072	µg/l	6/10/2019 14:11:03	
ICB1	S	Reactive	CN	P	0.3344	µg/l	6/10/2019 14:11:04	
CCV1	S	Reactive	CN	P	240.8927	µg/l	6/10/2019 14:11:05	
CCB1	S	Reactive	CN	P	0.3006	µg/l	6/10/2019 14:11:06	
PB120480BL	S	Reactive	CN	P	0.1243	µg/l	6/10/2019 14:11:07	
K3163-06	S	Reactive	CN	P	0.1661	µg/l	6/10/2019 14:11:08	
K3163-06DUP	S	Reactive	CN	P	0.0929	µg/l	6/10/2019 14:11:09	
K3163-08	S	Reactive	CN	P	0.0485	µg/l	6/10/2019 14:11:10	
K3265-09	S	Reactive	CN	P	-0.1365	µg/l	6/10/2019 14:11:11	
K3265-10	S	Reactive	CN	P	-0.0427	µg/l	6/10/2019 14:11:12	
K3265-11	S	Reactive	CN	P	-0.2099	µg/l	6/10/2019 14:11:13	
K3265-12	S	Reactive	CN	P	-0.6447	µg/l	6/10/2019 14:15:50	
K3262-01	S	Reactive	CN	P	-0.1319	µg/l	6/10/2019 14:15:51	
CCV2	S	Reactive	CN	P	254.4353	µg/l	6/10/2019 14:15:53	
CCB2	S	Reactive	CN	P	0.0891	µg/l	6/10/2019 14:15:54	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

Instrument ID : Konelab

6/10/2019 11:36


Test Total CN

Accepted 6/10/2019 11:36

Factor 989.1
 Bias 0.004

Coeff. of det. 0.999989

Errors

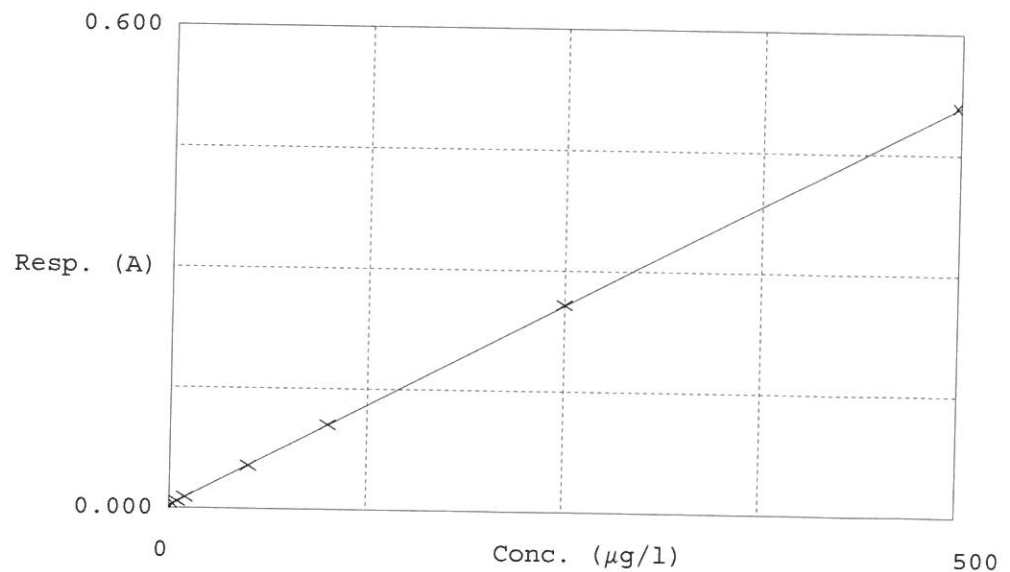

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.1135	0.0000	
2	5.0PPBCN	0.009	4.8579	5.0000	
3	10PPBCN	0.014	9.8534	10.0000	
4	50PPBCN	0.054	49.3451	50.0000	
5	100PPBCN	0.105	100.5933	100.0000	
6	250PPBCN	0.257	251.0253	250.0000	
7	500PPBCN	0.509	499.4385	500.0000	