

LB/03412

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/14/2019 13:12

Test: *Acetone*
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.165	0.0	0.104	
ICB1	-0.318	0.0	0.004	
CCV1	242.037	0.0	0.255	
CCB1	-0.427	0.0	0.004	
K3351-02	-0.547	0.0	0.004	
K3351-02DUP	-0.638	0.0	0.004	
K3351-04	-0.595	0.0	0.004	
K3351-06	-0.263	0.0	0.004	
K3351-08	-0.183	0.0	0.004	
K3352-02	-0.605	0.0	0.004	
K3352-04	-0.644	0.0	0.004	
K3366-02	-0.515	0.0	0.004	
K3368-01	-0.638	0.0	0.004	
CCV2	240.259	0.0	0.253	
CCB2	-0.516	0.0	0.004	
K3370-01	-0.515	0.0	0.004	
PB120623BL	-0.689	0.0	0.004	
K3369-02	-0.536	0.0	0.004	
K3369-02DUP	-0.647	0.0	0.004	
CCV3	239.752	0.0	0.252	
CCB3	-1.008	0.0	0.003	
PB120622BL	-0.699	0.0	0.004	
CCV3	258.187	0.0	0.271	
CCB3	-0.121	0.0	0.004	

N 24
Mean 44.429
SD 93.7915
CV% 211.10

AS

Aquakem v. 7.2AQ1

Results from time period:

Fri Jun 14 10:40:07 2019

Fri Jun 14 13:12:32 2019

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.8884	µg/l	6/14/2019 10:40:07	
5.0PPBCN	A	Reactive CN	P	4.0109	µg/l	6/14/2019 10:40:08	
10PPBCN	A	Reactive CN	P	9.2674	µg/l	6/14/2019 10:40:09	
50PPBCN	A	Reactive CN	P	50.1716	µg/l	6/14/2019 10:40:10	
100PPBCN	A	Reactive CN	P	101.5714	µg/l	6/14/2019 10:40:11	
250PPBCN	A	Reactive CN	P	252.3479	µg/l	6/14/2019 10:40:12	
500PPBCN	A	Reactive CN	P	498.5192	µg/l	6/14/2019 10:40:13	
ICV1	S	Reactive CN	P	96.1654	µg/l	6/14/2019 12:41:00	
ICB1	S	Reactive CN	P	-0.3177	µg/l	6/14/2019 12:41:01	
CCV1	S	Reactive CN	P	242.0368	µg/l	6/14/2019 12:41:02	
CCB1	S	Reactive CN	P	-0.4273	µg/l	6/14/2019 12:41:03	
K3351-02	S	Reactive CN	P	-0.5472	µg/l	6/14/2019 12:41:05	
K3351-02DUP	S	Reactive CN	P	-0.6378	µg/l	6/14/2019 12:41:06	
K3351-04	S	Reactive CN	P	-0.5953	µg/l	6/14/2019 12:41:07	
K3351-06	S	Reactive CN	P	-0.2633	µg/l	6/14/2019 12:41:08	
K3351-08	S	Reactive CN	P	-0.1831	µg/l	6/14/2019 12:41:09	
K3352-02	S	Reactive CN	P	-0.6054	µg/l	6/14/2019 12:41:10	
K3352-04	S	Reactive CN	P	-0.644	µg/l	6/14/2019 12:48:35	
K3366-02	S	Reactive CN	P	-0.5154	µg/l	6/14/2019 12:48:36	
K3368-01	S	Reactive CN	P	-0.638	µg/l	6/14/2019 12:48:37	
CCV2	S	Reactive CN	P	240.2588	µg/l	6/14/2019 12:48:38	
CCB2	S	Reactive CN	P	-0.5164	µg/l	6/14/2019 12:48:39	
K3370-01	S	Reactive CN	P	-0.5152	µg/l	6/14/2019 12:48:40	
PB120623BL	S	Reactive CN	P	-0.6894	µg/l	6/14/2019 12:48:41	
K3369-02	S	Reactive CN	P	-0.5362	µg/l	6/14/2019 12:48:42	
K3369-02DUP	S	Reactive CN	P	-0.6472	µg/l	6/14/2019 12:48:43	
CCV3	S	Reactive CN	P	239.7519	µg/l	6/14/2019 12:48:45	
CCB3	S	Reactive CN	P	-1.0083	µg/l	6/14/2019 12:51:23	
PB120622BL	S	Reactive CN	P	-0.6994	µg/l	6/14/2019 13:12:30	
CCV3	S	Reactive CN	P	258.1867	µg/l	6/14/2019 13:12:31	
CCB3	S	Reactive CN	P	-0.1214	µg/l	6/14/2019 13:12:32	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/14/2019 10:40


Test Total CN

Accepted 6/14/2019 10:40

Factor 967.3
Bias 0.004

Coeff. of det. 0.999939

Errors

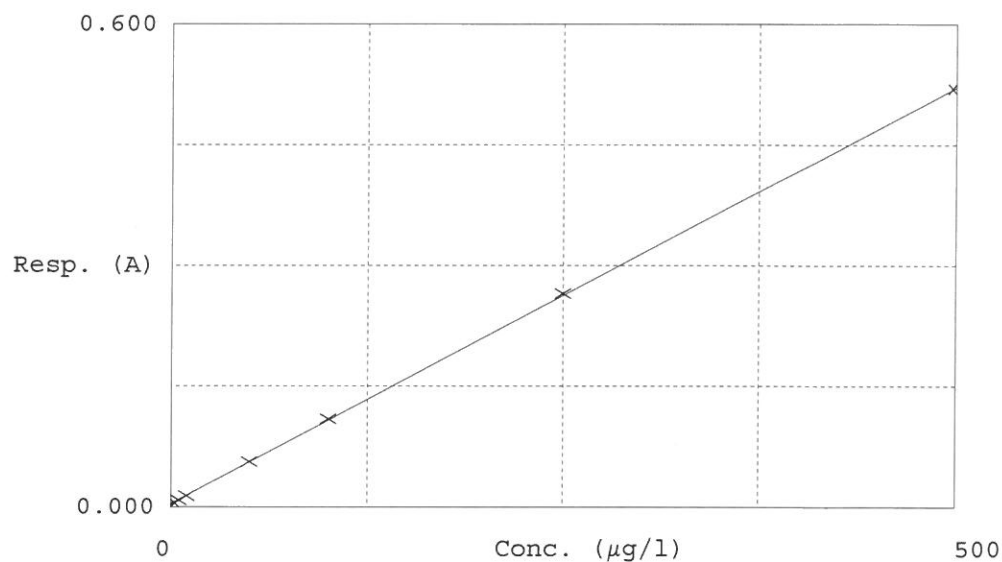

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.8884	0.0000	
2	5.0PPBCN	0.008	4.0109	5.0000	
3	10PPBCN	0.014	9.2674	10.0000	
4	50PPBCN	0.056	50.1716	50.0000	
5	100PPBCN	0.109	101.5714	100.0000	
6	250PPBCN	0.265	252.3479	250.0000	
7	500PPBCN	0.520	498.5192	500.0000	