

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/18/2019 12:54

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.904	0.0	0.101	
ICB1	-0.609	0.0	0.004	
CCV1	243.713	0.0	0.248	
CCB1	-0.918	0.0	0.004	
PB120678BL	-0.818	0.0	0.004	
K3154-02	-1.024	0.0	0.004	
K3154-02DUP	-0.896	0.0	0.004	
K3154-04	-1.024	0.0	0.004	
K3154-06	-0.972	0.0	0.004	
K3154-08	-1.022	0.0	0.004	
K3154-10	-0.947	0.0	0.004	
K3154-12	-0.714	0.0	0.004	
K3366-05	-0.347	0.0	0.004	
CCV2	246.154	0.0	0.250	
CCB2	-0.139	0.0	0.004	
K3389-08	0.369	0.0	0.005	
K3392-01	-0.324	0.0	0.004	
K3393-01	-1.104	0.0	0.004	
K3407-01	-0.769	0.0	0.004	
K3407-04	-0.788	0.0	0.004	
PB120679BL	-0.994	0.0	0.004	
K3382-03	-0.988	0.0	0.004	
K3382-03DUP	-0.951	0.0	0.004	
K3392-04	-0.793	0.0	0.004	
CCV3	244.193	0.0	0.248	
CCB3	-0.729	0.0	0.004	
PB120721BL	-0.914	0.0	0.004	
K3157-02	-0.809	0.0	0.004	
K3157-02DUP	-0.873	0.0	0.004	
K3157-04	-0.705	0.0	0.004	
K3157-06	-0.641	0.0	0.004	
K3157-08	-1.022	0.0	0.004	
K3157-10	-0.783	0.0	0.004	
K3158-04	-0.814	0.0	0.004	
K3163-10	-0.682	0.0	0.004	
K3163-12	-0.667	0.0	0.004	
CCV4	246.075	0.0	0.250	
CCB4	-0.589	0.0	0.004	
K3421-04	-0.576	0.0	0.004	
K3421-08	-0.678	0.0	0.004	
K3154-14	-0.612	0.0	0.004	
CCV5	244.797	0.0	0.249	
CCB5	-1.251	0.0	0.003	

N	43
Mean	30.086
SD	80.2656
CV%	266.78

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 18 12:21:41 2019

Tue Jun 18 12:47:11 2019

AS

Sample Id	Sam/Ctr/cf	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-1.2615	µg/l	6/18/2019 9:31:59	
5.OPPBCN	A	Reactive CN	P	3.908	µg/l	6/18/2019 9:32:00	
10PPBCN	A	Reactive CN	P	9.4156	µg/l	6/18/2019 9:32:01	
50PPBCN	A	Reactive CN	P	50.2943	µg/l	6/18/2019 9:32:02	
100PPBCN	A	Reactive CN	P	102.4071	µg/l	6/18/2019 9:32:03	
250PPBCN	A	Reactive CN	P	251.4493	µg/l	6/18/2019 9:32:04	
500PPBCN	A	Reactive CN	P	498.7871	µg/l	6/18/2019 9:32:05	
ICV1	S	Reactive CN	P	96.9043	µg/l	6/18/2019 12:21:41	
ICB1	S	Reactive CN	P	-0.6091	µg/l	6/18/2019 12:21:42	
CCV1	S	Reactive CN	P	243.713	µg/l	6/18/2019 12:21:43	
CCB1	S	Reactive CN	P	-0.918	µg/l	6/18/2019 12:21:44	
PB120678BL	S	Reactive CN	P	-0.8185	µg/l	6/18/2019 12:21:45	
K3154-02	S	Reactive CN	P	-1.0236	µg/l	6/18/2019 12:21:46	
K3154-02DUP	S	Reactive CN	P	-0.8959	µg/l	6/18/2019 12:21:47	
K3154-04	S	Reactive CN	P	-1.0236	µg/l	6/18/2019 12:21:48	
K3154-06	S	Reactive CN	P	-0.9725	µg/l	6/18/2019 12:21:49	
K3154-08	S	Reactive CN	P	-1.0219	µg/l	6/18/2019 12:21:50	
K3154-10	S	Reactive CN	P	-0.9471	µg/l	6/18/2019 12:21:51	
K3154-12	S	Reactive CN	P	-0.7142	µg/l	6/18/2019 12:29:16	
K3366-05	S	Reactive CN	P	-0.3466	µg/l	6/18/2019 12:29:18	
CCV2	S	Reactive CN	P	246.1541	µg/l	6/18/2019 12:29:19	
CCB2	S	Reactive CN	P	-0.1394	µg/l	6/18/2019 12:29:20	
K3389-08	S	Reactive CN	P	0.3689	µg/l	6/18/2019 12:29:21	
K3392-01	S	Reactive CN	P	-0.3238	µg/l	6/18/2019 12:29:22	
K3393-01	S	Reactive CN	P	-1.1038	µg/l	6/18/2019 12:29:24	
K3407-01	S	Reactive CN	P	-0.7686	µg/l	6/18/2019 12:29:25	
K3407-04	S	Reactive CN	P	-0.7877	µg/l	6/18/2019 12:29:26	
PB120679BL	S	Reactive CN	P	-0.9937	µg/l	6/18/2019 12:36:48	
K3382-03	S	Reactive CN	P	-0.9882	µg/l	6/18/2019 12:36:49	
K3382-03DUP	S	Reactive CN	P	-0.9514	µg/l	6/18/2019 12:36:50	
K3392-04	S	Reactive CN	P	-0.7931	µg/l	6/18/2019 12:36:51	
CCV3	S	Reactive CN	P	244.1927	µg/l	6/18/2019 12:36:52	
CCB3	S	Reactive CN	P	-0.7295	µg/l	6/18/2019 12:36:53	
PB120721BL	S	Reactive CN	P	-0.9139	µg/l	6/18/2019 12:36:54	
K3157-02	S	Reactive CN	P	-0.8094	µg/l	6/18/2019 12:36:55	
K3157-02DUP	S	Reactive CN	P	-0.8734	µg/l	6/18/2019 12:36:56	
K3157-04	S	Reactive CN	P	-0.7048	µg/l	6/18/2019 12:36:57	
K3157-06	S	Reactive CN	P	-0.6413	µg/l	6/18/2019 12:36:58	
K3157-08	S	Reactive CN	P	-1.0215	µg/l	6/18/2019 12:44:23	
K3157-10	S	Reactive CN	P	-0.7826	µg/l	6/18/2019 12:44:24	
K3158-04	S	Reactive CN	P	-0.8136	µg/l	6/18/2019 12:44:25	
K3163-10	S	Reactive CN	P	-0.6821	µg/l	6/18/2019 12:44:26	

AS

K3163-12	S	Reactive CN	P	-0.6667 µg/l	6/18/2019 12:44:27
CCV4	S	Reactive CN	P	246.0753 µg/l	6/18/2019 12:44:28
CCB4	S	Reactive CN	P	-0.5893 µg/l	6/18/2019 12:44:29
K3421-04	S	Reactive CN	P	-0.576 µg/l	6/18/2019 12:44:30
K3421-08	S	Reactive CN	P	-0.6784 µg/l	6/18/2019 12:44:31
K3154-14	S	Reactive CN	P	-0.6116 µg/l	6/18/2019 12:44:32
CCV5	S	Reactive CN	P	244.7968 µg/l	6/18/2019 12:44:33
CCB5	S	Reactive CN	P	-1.2511 µg/l	6/18/2019 12:47:11

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/18/2019 9:36


Test Total CN

Accepted 6/18/2019 9:36

Factor 1002
Bias 0.005

Coeff. of det. 0.999939

Errors

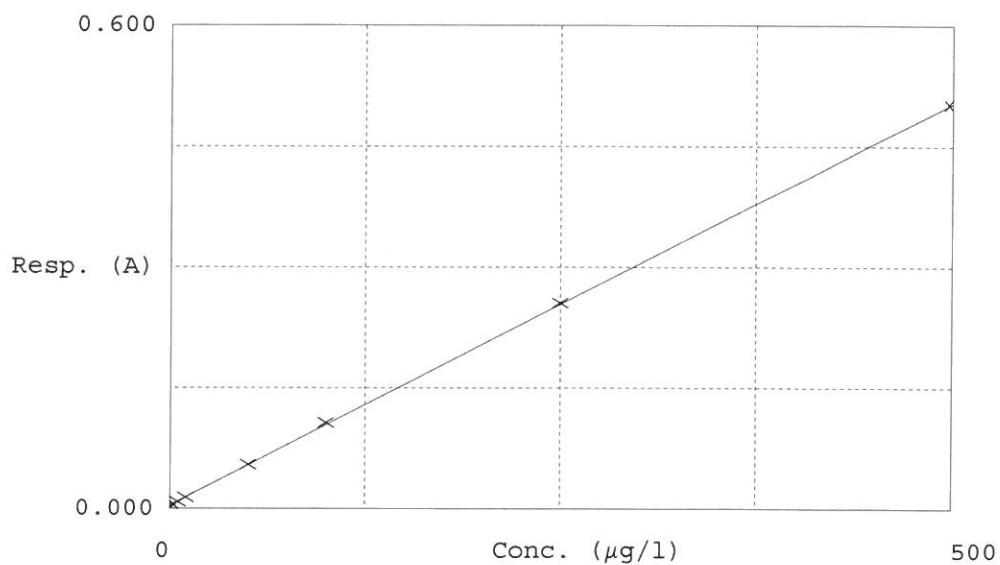

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.2615	0.0000	
2	5.0PPBCN	0.009	3.9080	5.0000	
3	10PPBCN	0.014	9.4156	10.0000	
4	50PPBCN	0.055	50.2943	50.0000	
5	100PPBCN	0.107	102.4071	100.0000	
6	250PPBCN	0.256	251.4493	250.0000	
7	500PPBCN	0.502	498.7871	500.0000	