

213103579

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/24/2019 11:11

Test: *Reactive*
~~Total~~ CN

Mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	90.690	0.0	0.100	
ICB1	-0.869	0.0	0.004	
CCV1	234.824	0.0	0.251	
CCB1	-1.180	0.0	0.004	
PB120821BL	-1.324	0.0	0.004	
K3158-06	-1.359	0.0	0.004	
K3158-06DUP	-1.258	0.0	0.004	
K3470-04	-1.326	0.0	0.004	
K3470-08	-1.227	0.0	0.004	
K3470-12	-1.219	0.0	0.004	
CCV2	237.502	0.0	0.254	
CCB2	-1.191	0.0	0.004	

N	12
Mean	46.005
SD	92.6332
CV%	201.35

Aquakem v. 7.2AQ1

Results from time period:

Mon Jun 24 11:06:09 2019

Mon Jun 24 11:08:57 2019

AS

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-1.3815	µg/l	6/24/2019 8:45:05	
5.0PPBCN	A	Reactive CN	P	3.936	µg/l	6/24/2019 8:45:06	
10PPBCN	A	Reactive CN	P	9.909	µg/l	6/24/2019 8:45:07	
50PPBCN	A	Reactive CN	P	50.05	µg/l	6/24/2019 8:45:08	
100PPBCN	A	Reactive CN	P	99.247	µg/l	6/24/2019 8:45:09	
250PPBCN	A	Reactive CN	P	256.163	µg/l	6/24/2019 8:45:10	
500PPBCN	A	Reactive CN	P	497.0766	µg/l	6/24/2019 8:45:11	
ICV1	S	Reactive CN	P	90.69	µg/l	6/24/2019 11:06:09	
ICB1	S	Reactive CN	P	-0.8692	µg/l	6/24/2019 11:06:10	
CCV1	S	Reactive CN	P	234.8237	µg/l	6/24/2019 11:06:11	
CCB1	S	Reactive CN	P	-1.1804	µg/l	6/24/2019 11:06:12	
PB120821BL	S	Reactive CN	P	-1.3243	µg/l	6/24/2019 11:06:13	
K3158-06	S	Reactive CN	P	-1.3588	µg/l	6/24/2019 11:06:14	
K3158-06DUP	S	Reactive CN	P	-1.2583	µg/l	6/24/2019 11:06:15	
K3470-04	S	Reactive CN	P	-1.326	µg/l	6/24/2019 11:06:16	
K3470-08	S	Reactive CN	P	-1.227	µg/l	6/24/2019 11:06:17	
K3470-12	S	Reactive CN	P	-1.2188	µg/l	6/24/2019 11:06:18	
CCV2	S	Reactive CN	P	237.5022	µg/l	6/24/2019 11:06:19	
CCB2	S	Reactive CN	P	-1.1909	µg/l	6/24/2019 11:08:57	

=====

Calibration results	Aquakem 7.2AQ1	Page: 1
---------------------	----------------	---------

6/24/2019 8:46

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS Instrument ID : Konelab


Test Total CN

Accepted 6/24/2019 8:46

Factor 954.8
Bias 0.005

Coeff. of det. 0.999756

Errors

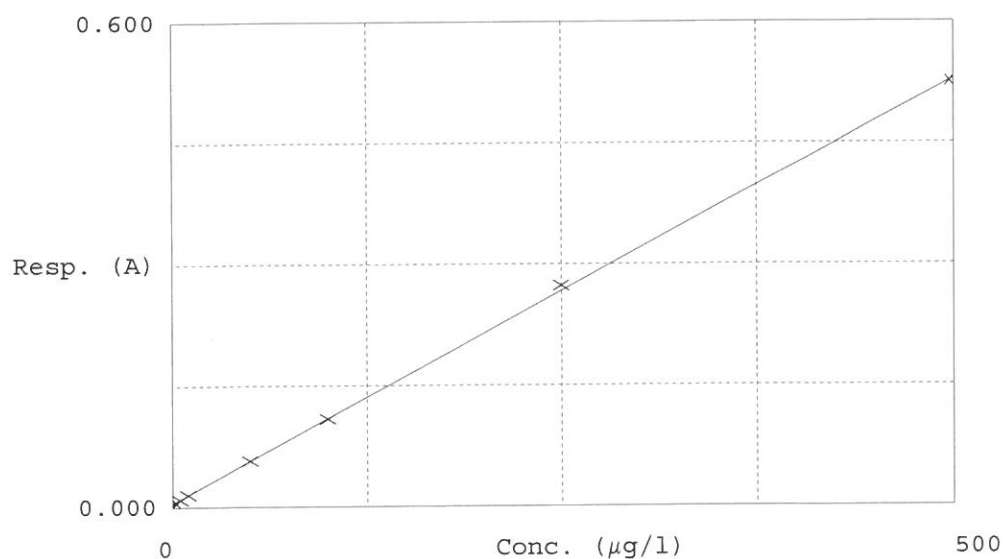

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-1.3815	0.0000	
2	5.0PPBCN	0.009	3.9360	5.0000	
3	10PPBCN	0.015	9.9090	10.0000	
4	50PPBCN	0.057	50.0500	50.0000	
5	100PPBCN	0.109	99.2470	100.0000	
6	250PPBCN	0.273	256.1630	250.0000	
7	500PPBCN	0.526	497.0766	500.0000	