

2B/03609

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/25/2019 12:08

Test: Dechlorine
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.405	0.0	0.105	
ICB1	-0.405	0.0	0.003	
CCV1	245.912	0.0	0.258	
CCB1	-0.521	0.0	0.002	
PB120886BL	-0.727	0.0	0.002	
K3156-06	-0.724	0.0	0.002	
K3156-06DUP	-0.663	0.0	0.002	
K3503-01	-0.706	0.0	0.002	
K3510-02	-0.840	0.0	0.002	
K3511-02	-0.925	0.0	0.002	
K3511-04	-0.830	0.0	0.002	
K3512-04	-0.753	0.0	0.002	
K3512-08	-1.082	0.0	0.002	
PB120887BL	-0.940	0.0	0.002	
CCV2	261.363	0.0	0.274	
CCB2	-0.275	0.0	0.003	
K3511-06	-0.995	0.0	0.002	
K3511-06DUP	-1.027	0.0	0.002	
CCV3	258.626	0.0	0.271	
CCB3	-0.467	0.0	0.003	

N	20
Mean	42.621
SD	94.3208
CV%	221.30

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 25 09:41:26 2019

Tue Jun 25 12:05:43 2019



Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-1.0086	µg/l	6/25/2019 11:22:42	
5.OPPBCN	A	Reactive CN	P	4.1605	µg/l	6/25/2019 11:22:43	
10PPBCN	A	Reactive CN	P	9.4511	µg/l	6/25/2019 11:22:44	
50PPBCN	A	Reactive CN	P	49.9584	µg/l	6/25/2019 11:22:45	
100PPBCN	A	Reactive CN	P	101.8779	µg/l	6/25/2019 11:22:46	
250PPBCN	A	Reactive CN	P	251.8255	µg/l	6/25/2019 11:22:47	
500PPBCN	A	Reactive CN	P	498.7352	µg/l	6/25/2019 11:22:48	
ICV1	S	Reactive CN	P	98.4055	µg/l	6/25/2019 11:54:48	
ICB1	S	Reactive CN	P	-0.4051	µg/l	6/25/2019 11:54:49	
CCV1	S	Reactive CN	P	245.9116	µg/l	6/25/2019 11:54:50	
CCB1	S	Reactive CN	P	-0.5207	µg/l	6/25/2019 11:54:51	
PB120886BL	S	Reactive CN	P	-0.727	µg/l	6/25/2019 11:54:52	
K3156-06	S	Reactive CN	P	-0.7238	µg/l	6/25/2019 11:54:53	
K3156-06DUP	S	Reactive CN	P	-0.6625	µg/l	6/25/2019 11:54:54	
K3503-01	S	Reactive CN	P	-0.7057	µg/l	6/25/2019 11:54:55	
K3510-02	S	Reactive CN	P	-0.8404	µg/l	6/25/2019 11:54:56	
K3511-02	S	Reactive CN	P	-0.9252	µg/l	6/25/2019 11:54:57	
K3511-04	S	Reactive CN	P	-0.8296	µg/l	6/25/2019 11:54:58	
K3512-04	S	Reactive CN	P	-0.7531	µg/l	6/25/2019 11:59:35	
K3512-08	S	Reactive CN	P	-1.0816	µg/l	6/25/2019 11:59:36	
PB120887BL	S	Reactive CN	P	-0.9402	µg/l	6/25/2019 11:59:37	
CCV2	S	Reactive CN	P	261.3628	µg/l	6/25/2019 11:59:38	
CCB2	S	Reactive CN	P	-0.2746	µg/l	6/25/2019 11:59:39	
K3511-06	S	Reactive CN	P	-0.9949	µg/l	6/25/2019 12:05:39	
K3511-06DUP	S	Reactive CN	P	-1.0267	µg/l	6/25/2019 12:05:40	
CCV3	S	Reactive CN	P	258.6257	µg/l	6/25/2019 12:05:42	
CCB3	S	Reactive CN	P	-0.4665	µg/l	6/25/2019 12:05:43	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ, 07092
Reviewed by : AS

Instrument ID : Konelab

6/25/2019 11:24


Test Total CN

Accepted 6/25/2019 11:24

Factor 964.8
Bias 0.003

Coeff. of det. 0.999949

Errors

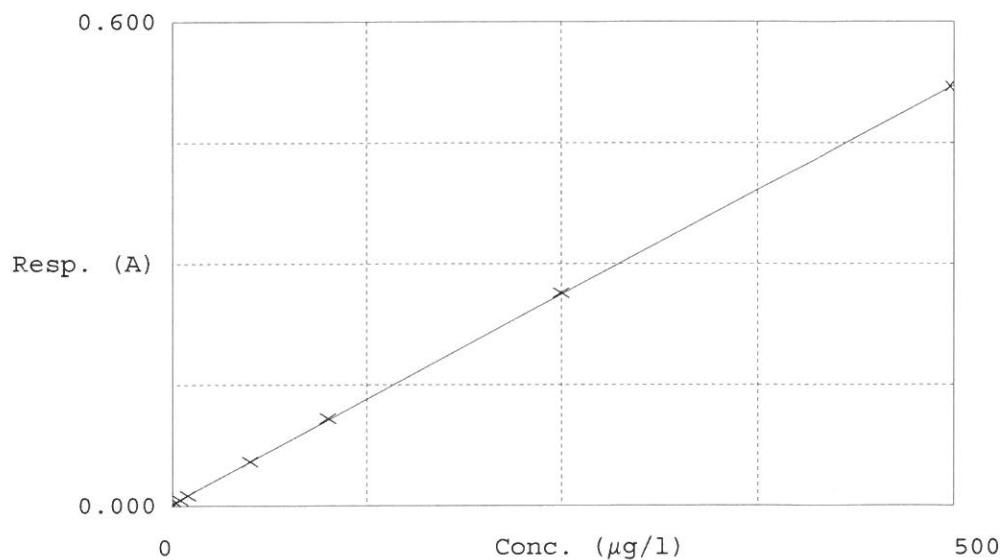

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-1.0086	0.0000	
2	5.0PPBCN	0.007	4.1605	5.0000	
3	10PPBCN	0.013	9.4511	10.0000	
4	50PPBCN	0.055	49.9584	50.0000	
5	100PPBCN	0.109	101.8779	100.0000	
6	250PPBCN	0.264	251.8255	250.0000	
7	500PPBCN	0.520	498.7352	500.0000	