

2B103859

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

7/9/2019 13:13

Test: ^{Reactive} ~~Total~~ CN

Hg/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.907	0.0	0.092	
ICB1	-0.129	0.0	0.001	
CCV1	247.432	0.0	0.229	
CCB1	-0.204	0.0	0.001	
PB121238BL	-0.377	0.0	0.001	
K3627-02	-0.497	0.0	0.001	
K3627-02DUP	-0.471	0.0	0.001	
K3687-07	-0.156	0.0	0.001	
K3687-08	-0.105	0.0	0.001	
K3693-02	-0.206	0.0	0.001	
K3694-08	-0.319	0.0	0.001	
K3695-01	-0.056	0.0	0.001	
K3695-02	-0.056	0.0	0.001	
K3695-03	-0.027	0.0	0.001	
CCV2	249.981	0.0	0.231	
CCB2	0.024	0.0	0.001	
K3697-03	-0.068	0.0	0.001	
K3697-06	-0.039	0.0	0.001	
CCV3	252.491	0.0	0.234	
CCB3	0.279	0.0	0.002	

N 20
Mean 42.320
SD 92.1750
CV% 217.80

Aquakem v. 7.2AQ1

Results from time period:

Tue Jul 09 13:04:31 2019

Tue Jul 09 13:11:47 2019

✓ AS

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.4176	µg/l	7/9/2019 11:21:50	
5.0PPBCN	A	Reactive CN	P	4.0704	µg/l	7/9/2019 11:21:51	
10PPBCN	A	Reactive CN	P	9.7049	µg/l	7/9/2019 11:21:52	
50PPBCN	A	Reactive CN	P	51.865	µg/l	7/9/2019 11:21:53	
100PPBCN	A	Reactive CN	P	100.1881	µg/l	7/9/2019 11:21:54	
250PPBCN	A	Reactive CN	P	247.9258	µg/l	7/9/2019 11:21:55	
500PPBCN	A	Reactive CN	P	500.8282	µg/l	7/9/2019 11:21:56	
ICV1	S	Reactive CN	P	98.9071	µg/l	7/9/2019 13:04:31	
ICB1	S	Reactive CN	P	-0.1293	µg/l	7/9/2019 13:04:32	
CCV1	S	Reactive CN	P	247.4323	µg/l	7/9/2019 13:04:33	
CCB1	S	Reactive CN	P	-0.2039	µg/l	7/9/2019 13:04:34	
PB121238BL	S	Reactive CN	P	-0.3769	µg/l	7/9/2019 13:04:35	
K3627-02	S	Reactive CN	P	-0.497	µg/l	7/9/2019 13:04:36	
K3627-02DUP	S	Reactive CN	P	-0.4709	µg/l	7/9/2019 13:04:37	
K3687-07	S	Reactive CN	P	-0.1562	µg/l	7/9/2019 13:04:38	
K3687-08	S	Reactive CN	P	-0.1053	µg/l	7/9/2019 13:04:39	
K3693-02	S	Reactive CN	P	-0.2064	µg/l	7/9/2019 13:04:40	
K3694-08	S	Reactive CN	P	-0.3187	µg/l	7/9/2019 13:04:41	
K3695-01	S	Reactive CN	P	-0.0563	µg/l	7/9/2019 13:11:38	
K3695-02	S	Reactive CN	P	-0.0555	µg/l	7/9/2019 13:11:39	
K3695-03	S	Reactive CN	P	-0.0272	µg/l	7/9/2019 13:11:40	
CCV2	S	Reactive CN	P	249.9811	µg/l	7/9/2019 13:11:41	
CCB2	S	Reactive CN	P	0.0245	µg/l	7/9/2019 13:11:42	
K3697-03	S	Reactive CN	P	-0.0683	µg/l	7/9/2019 13:11:43	
K3697-06	S	Reactive CN	P	-0.0394	µg/l	7/9/2019 13:11:44	
CCV3	S	Reactive CN	P	252.4908	µg/l	7/9/2019 13:11:46	
CCB3	S	Reactive CN	P	0.2789	µg/l	7/9/2019 13:11:47	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

7/9/2019 11:26


Test Total CN

Accepted 7/9/2019 11:26

Factor 1087
Bias 0.001

Coeff. of det. 0.999953

Errors

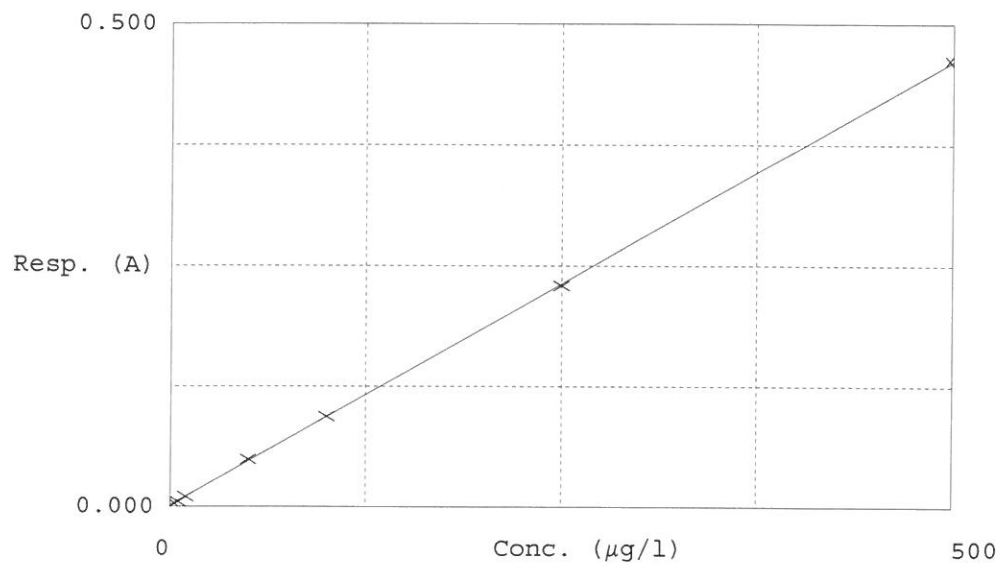

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.4176	0.0000	
2	5.0PPBCN	0.005	4.0704	5.0000	
3	10PPBCN	0.010	9.7049	10.0000	
4	50PPBCN	0.049	51.8650	50.0000	
5	100PPBCN	0.094	100.1881	100.0000	
6	250PPBCN	0.230	247.9258	250.0000	
7	500PPBCN	0.462	500.8282	500.0000	