

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AS

Instrument ID : Konelab

7/9/2019 14:07

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	99.013	0.0	0.093	
ICB1	0.019	0.0	0.001	
CCV1	248.560	0.0	0.230	
CCB1	-0.199	0.0	0.001	
PB121234BL	0.090	0.0	0.002	
PB121234BS	99.845	0.0	0.093	
LOWPB121234	10.441	0.0	0.011	
HIGHPB121234	501.749	0.0	0.463	Test limit high
K3627-01	0.792	0.0	0.002	
K3627-01DUP	0.294	0.0	0.002	
K3627-01MS	37.356	0.0	0.036	
K3627-01MSD	36.538	0.0	0.035	
K3687-03	1.857	0.0	0.003	
K3693-01	0.378	0.0	0.002	
CCV2	248.811	0.0	0.230	
CCB2	-0.294	0.0	0.001	
K3697-04	0.591	0.0	0.002	
K3699-01	0.070	0.0	0.001	
K3700-01	0.203	0.0	0.002	
K3703-01	1.000	0.0	0.002	
K3694-01	2.838	0.0	0.004	
K3697-01	0.249	0.0	0.002	
PB121235BL	-0.141	0.0	0.001	
PB121235BS	100.931	0.0	0.094	
K3591-03	1.121	0.0	0.002	
K3591-09	1.174	0.0	0.003	
CCV3	256.843	0.0	0.238	
CCB3	0.099	0.0	0.002	

N	28
Mean	58.937
SD	118.1597
CV%	200.49

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : _____

Instrument ID : Konelab

7/9/2019 11:26


Test Total CN

Accepted 7/9/2019 11:26

Factor 1087
Bias 0.001

Coeff. of det. 0.999953

Errors

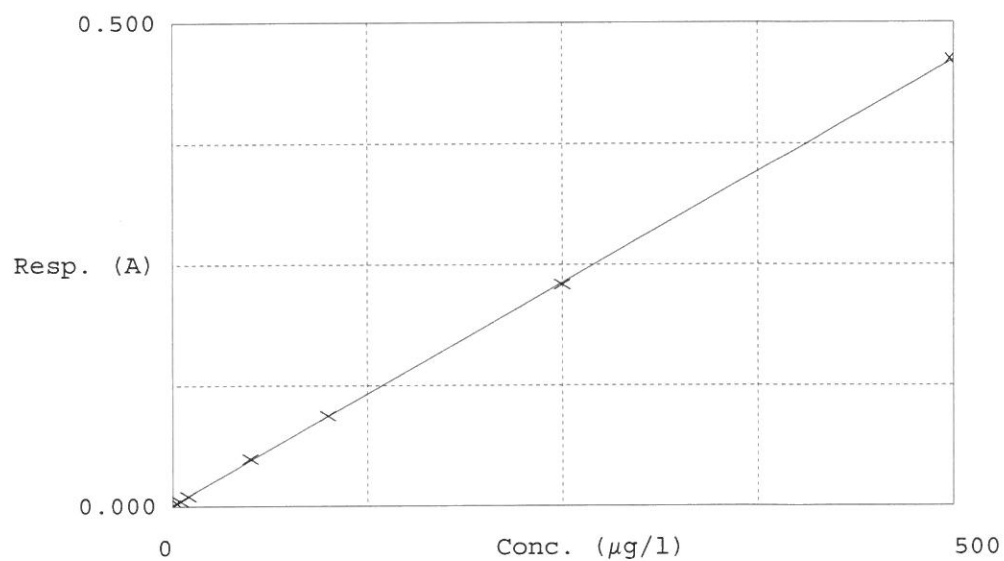

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.4176	0.0000	
2	5.0PPBCN	0.005	4.0704	5.0000	
3	10PPBCN	0.010	9.7049	10.0000	
4	50PPBCN	0.049	51.8650	50.0000	
5	100PPBCN	0.094	100.1881	100.0000	
6	250PPBCN	0.230	247.9258	250.0000	
7	500PPBCN	0.462	500.8282	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Tue Jul 09 13:46:52 2019

Tue Jul 09 14:00:45 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.4176	µg/l	7/9/2019 11:21:50	
5.0PPBCN	A	Total CN	P	4.0704	µg/l	7/9/2019 11:21:51	
10PPBCN	A	Total CN	P	9.7049	µg/l	7/9/2019 11:21:52	
50PPBCN	A	Total CN	P	51.865	µg/l	7/9/2019 11:21:53	
100PPBCN	A	Total CN	P	100.1881	µg/l	7/9/2019 11:21:54	
250PPBCN	A	Total CN	P	247.9258	µg/l	7/9/2019 11:21:55	
500PPBCN	A	Total CN	P	500.8282	µg/l	7/9/2019 11:21:56	
ICV1	S	Total CN	P	99.0126	µg/l	7/9/2019 13:46:52	
ICB1	S	Total CN	P	0.0193	µg/l	7/9/2019 13:46:53	
CCV1	S	Total CN	P	248.5602	µg/l	7/9/2019 13:46:54	
CCB1	S	Total CN	P	-0.1993	µg/l	7/9/2019 13:46:55	
PB121234BL	S	Total CN	P	0.0903	µg/l	7/9/2019 13:46:56	
PB121234BS	S	Total CN	P	99.8449	µg/l	7/9/2019 13:46:57	
LOWPB121234	S	Total CN	P	10.4412	µg/l	7/9/2019 13:46:58	
HIGHPB121234	S	Total CN	P	501.7489	µg/l	7/9/2019 13:46:59	
K3627-01	S	Total CN	P	0.792	µg/l	7/9/2019 13:47:00	
K3627-01DUP	S	Total CN	P	0.2937	µg/l	7/9/2019 13:47:01	
K3627-01MS	S	Total CN	P	37.3559	µg/l	7/9/2019 13:47:02	
K3627-01MSD	S	Total CN	P	36.5378	µg/l	7/9/2019 13:54:27	
K3687-03	S	Total CN	P	1.8566	µg/l	7/9/2019 13:54:28	
K3693-01	S	Total CN	P	0.3785	µg/l	7/9/2019 13:54:29	
CCV2	S	Total CN	P	248.8113	µg/l	7/9/2019 13:54:30	
CCB2	S	Total CN	P	-0.2939	µg/l	7/9/2019 13:54:31	
K3697-04	S	Total CN	P	0.5914	µg/l	7/9/2019 13:54:32	
K3699-01	S	Total CN	P	0.0702	µg/l	7/9/2019 13:54:33	
K3700-01	S	Total CN	P	0.2034	µg/l	7/9/2019 13:54:34	
K3703-01	S	Total CN	P	0.9996	µg/l	7/9/2019 13:54:35	
K3694-01	S	Total CN	P	2.8376	µg/l	7/9/2019 13:54:36	
K3697-01	S	Total CN	P	0.2485	µg/l	7/9/2019 13:54:37	
PB121235BL	S	Total CN	P	-0.1411	µg/l	7/9/2019 14:00:38	
PB121235BS	S	Total CN	P	100.9305	µg/l	7/9/2019 14:00:39	
K3591-03	S	Total CN	P	1.1205	µg/l	7/9/2019 14:00:42	
K3591-09	S	Total CN	P	1.1744	µg/l	7/9/2019 14:00:43	
CCV3	S	Total CN	P	256.8428	µg/l	7/9/2019 14:00:44	
CCB3	S	Total CN	P	0.0988	µg/l	7/9/2019 14:00:45	