

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

7/12/2019 14:00

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.533	0.0	0.084	
ICB1	0.540	0.0	0.002	
CCV1	248.345	0.0	0.218	
CCB1	0.310	0.0	0.002	
PB121311BL	0.388	0.0	0.002	
K3621-02	0.286	0.0	0.001	
K3621-02DUP	0.349	0.0	0.002	
K3621-04	0.026	0.0	0.001	
K3740-07	0.204	0.0	0.001	
K3740-08	0.152	0.0	0.001	
K3740-09	0.225	0.0	0.001	
PB121333BL	0.217	0.0	0.001	
K3618-04	0.243	0.0	0.001	
CCV2	248.225	0.0	0.217	
CCB2	-0.132	0.0	0.001	
K3626-06	0.168	0.0	0.001	
K3626-08	0.096	0.0	0.001	
K3761-02	0.190	0.0	0.001	
K3618-04DUP	0.226	0.0	0.001	
CCV3	261.872	0.0	0.229	
CCB3	0.470	0.0	0.002	

N	21
Mean	40.806
SD	91.0597
CV%	223.15

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AS

Instrument ID : Konelab

7/12/2019 11:33


Test Total CN

Accepted 7/12/2019 11:33

Factor 1148
Bias 0.001

Coeff. of det. 0.999963

Errors

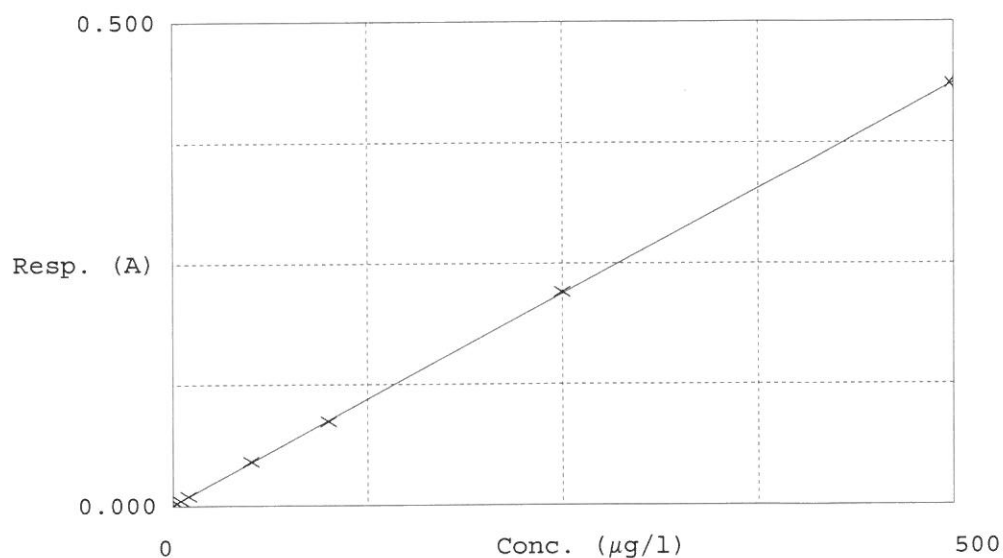

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.6859	0.0000	
2	5.0PPBCN	0.006	4.9129	5.0000	
3	10PPBCN	0.010	10.1639	10.0000	
4	50PPBCN	0.046	51.1243	50.0000	
5	100PPBCN	0.087	98.4261	100.0000	
6	250PPBCN	0.220	251.7174	250.0000	
7	500PPBCN	0.436	499.3412	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri Jul 12 13:12:06 2019

Fri Jul 12 13:58:22 2019

✓ AS

Sample Id	Sam/Ctr/c/	Test short	nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	CN	P	-0.6859	µg/l	7/12/2019 11:30:14	
5.OPPBCN	A	Reactive	CN	P	4.9129	µg/l	7/12/2019 11:30:15	
10PPBCN	A	Reactive	CN	P	10.1639	µg/l	7/12/2019 11:30:16	
50PPBCN	A	Reactive	CN	P	51.1243	µg/l	7/12/2019 11:30:17	
100PPBCN	A	Reactive	CN	P	98.4261	µg/l	7/12/2019 11:30:18	
250PPBCN	A	Reactive	CN	P	251.7174	µg/l	7/12/2019 11:30:19	
500PPBCN	A	Reactive	CN	P	499.3412	µg/l	7/12/2019 11:30:20	
ICV1	S	Reactive	CN	P	94.5328	µg/l	7/12/2019 13:12:06	
ICB1	S	Reactive	CN	P	0.5396	µg/l	7/12/2019 13:12:07	
CCV1	S	Reactive	CN	P	248.3448	µg/l	7/12/2019 13:12:08	
CCB1	S	Reactive	CN	P	0.3103	µg/l	7/12/2019 13:12:09	
PB121311BL	S	Reactive	CN	P	0.3878	µg/l	7/12/2019 13:12:10	
K3621-02	S	Reactive	CN	P	0.2859	µg/l	7/12/2019 13:12:11	
K3621-02DUP	S	Reactive	CN	P	0.3495	µg/l	7/12/2019 13:12:12	
K3621-04	S	Reactive	CN	P	0.0256	µg/l	7/12/2019 13:12:13	
K3740-07	S	Reactive	CN	P	0.2041	µg/l	7/12/2019 13:12:14	
K3740-08	S	Reactive	CN	P	0.1523	µg/l	7/12/2019 13:12:15	
K3740-09	S	Reactive	CN	P	0.2254	µg/l	7/12/2019 13:12:16	
PB121333BL	S	Reactive	CN	P	0.2168	µg/l	7/12/2019 13:19:41	
K3618-04	S	Reactive	CN	P	0.2431	µg/l	7/12/2019 13:19:42	
CCV2	S	Reactive	CN	P	248.2253	µg/l	7/12/2019 13:38:21	
CCB2	S	Reactive	CN	P	-0.1317	µg/l	7/12/2019 13:38:22	
K3626-06	S	Reactive	CN	P	0.1679	µg/l	7/12/2019 13:38:23	
K3626-08	S	Reactive	CN	P	0.0956	µg/l	7/12/2019 13:38:24	
K3761-02	S	Reactive	CN	P	0.1901	µg/l	7/12/2019 13:38:25	
K3618-04DUP	S	Reactive	CN	P	0.226	µg/l	7/12/2019 13:58:20	
CCV3	S	Reactive	CN	P	261.8721	µg/l	7/12/2019 13:58:21	
CCB3	S	Reactive	CN	P	0.4698	µg/l	7/12/2019 13:58:22	