

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : CT

Instrument ID : Konelab

7/31/2019 8:37


Test ~~Total~~ ^{Reactive} CN

Accepted 7/31/2019 8:37

Factor 1089
 Bias 0.001

Coeff. of det. 0.999911

Errors

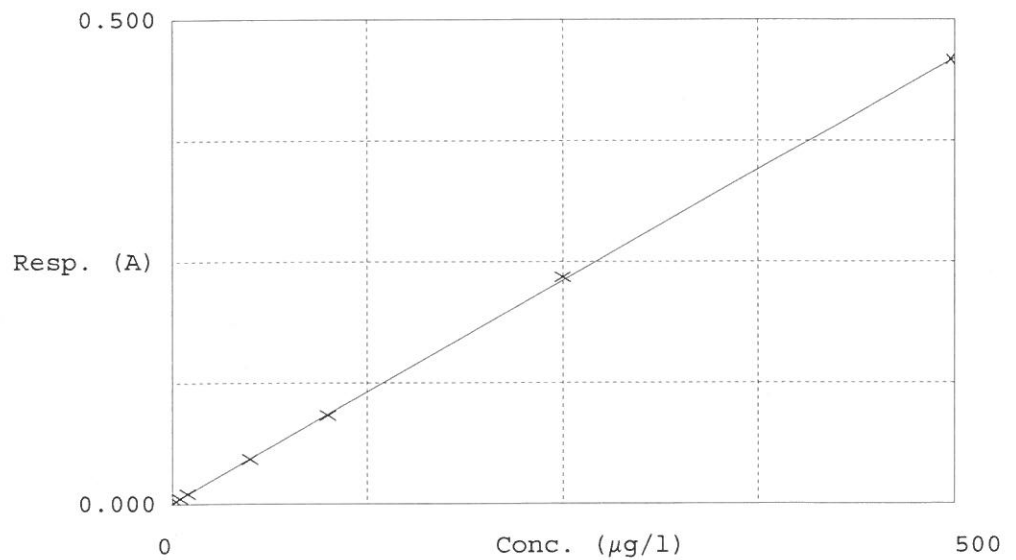

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.4752	0.0000	
2	5.0PPBCN	0.006	4.9488	5.0000	
3	10PPBCN	0.011	10.3018	10.0000	
4	50PPBCN	0.047	49.4770	50.0000	
5	100PPBCN	0.092	98.5867	100.0000	
6	250PPBCN	0.234	253.6631	250.0000	
7	500PPBCN	0.459	498.4979	500.0000	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

7/31/2019 9:15

Test: ~~Total~~ ^{Reactive} CNug/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.634	0.0	0.088	
ICB1	0.313	0.0	0.001	
CCV1	242.082	0.0	0.223	
CCB1	0.645	0.0	0.002	
PB121805BL	1.098	0.0	0.002	
K3621-08	0.215	0.0	0.001	
K3621-08DUP	0.080	0.0	0.001	
K3622-14	0.019	0.0	0.001	
K3622-16	0.084	0.0	0.001	
K4044-04	0.042	0.0	0.001	
K4044-06	-0.059	0.0	0.001	
K4044-10	0.085	0.0	0.001	
K4044-16	0.090	0.0	0.001	
K4044-18	-0.075	0.0	0.001	
CCV2	249.772	0.0	0.230	
CCB2	-0.025	0.0	0.001	

N	16
Mean	36.813
SD	84.9566
CV%	230.78

CT
07/31/19

Aquakem v. 7.2AQ1

Results from time period:

Wed Jul 31 08:35:29 2019

Wed Jul 31 09:14:18 2019

CT

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.4752	µg/l	7/31/2019 8:35:29	
5.0PPBCN	A	Reactive CN	P	4.9488	µg/l	7/31/2019 8:35:30	
10PPBCN	A	Reactive CN	P	10.3018	µg/l	7/31/2019 8:35:31	
50PPBCN	A	Reactive CN	P	49.477	µg/l	7/31/2019 8:35:32	
100PPBCN	A	Reactive CN	P	98.5867	µg/l	7/31/2019 8:35:33	
250PPBCN	A	Reactive CN	P	253.6631	µg/l	7/31/2019 8:35:34	
500PPBCN	A	Reactive CN	P	498.4979	µg/l	7/31/2019 8:35:35	
ICV1	S	Reactive CN	P	94.6336	µg/l	7/31/2019 9:09:27	
ICB1	S	Reactive CN	P	0.313	µg/l	7/31/2019 9:09:28	
CCV1	S	Reactive CN	P	242.0818	µg/l	7/31/2019 9:09:29	
CCB1	S	Reactive CN	P	0.6452	µg/l	7/31/2019 9:09:30	
PB121805BL	S	Reactive CN	P	1.0985	µg/l	7/31/2019 9:09:31	
K3621-08	S	Reactive CN	P	0.2151	µg/l	7/31/2019 9:09:32	
K3621-08DUP	S	Reactive CN	P	0.0802	µg/l	7/31/2019 9:09:33	
K3622-14	S	Reactive CN	P	0.0193	µg/l	7/31/2019 9:09:34	
K3622-16	S	Reactive CN	P	0.0841	µg/l	7/31/2019 9:09:35	
K4044-04	S	Reactive CN	P	0.042	µg/l	7/31/2019 9:09:36	
K4044-06	S	Reactive CN	P	-0.0586	µg/l	7/31/2019 9:09:37	
K4044-10	S	Reactive CN	P	0.0853	µg/l	7/31/2019 9:14:14	
K4044-16	S	Reactive CN	P	0.0902	µg/l	7/31/2019 9:14:15	
K4044-18	S	Reactive CN	P	-0.0748	µg/l	7/31/2019 9:14:16	
CCV2	S	Reactive CN	P	249.7722	µg/l	7/31/2019 9:14:17	
CCB2	S	Reactive CN	P	-0.0251	µg/l	7/31/2019 9:14:18	