

LB104591

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : CT

Instrument ID : Konelab

8/14/2019 10:07


Test ^{Reactive}
~~Total~~ CN

Accepted 8/14/2019 10:07

Factor 1060
Bias 0.002

Coeff. of det. 0.999925

Errors

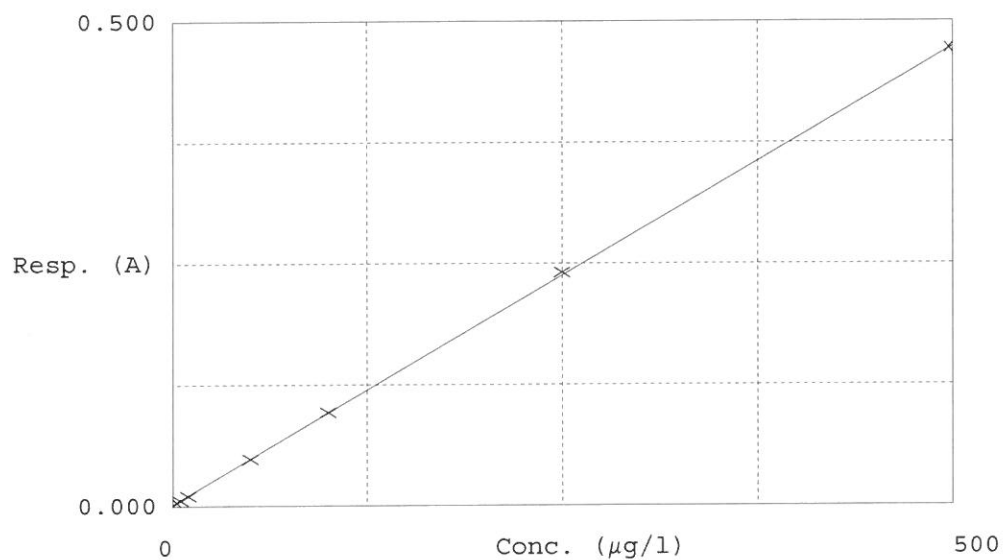

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.4428	0.0000	
2	5.0PPBCN	0.006	4.1344	5.0000	
3	10PPBCN	0.010	8.9764	10.0000	
4	50PPBCN	0.048	49.3379	50.0000	
5	100PPBCN	0.097	100.5278	100.0000	
6	250PPBCN	0.241	253.1819	250.0000	
7	500PPBCN	0.472	498.3988	500.0000	

CT
08/14/19

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

8/14/2019 12:03

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.234	0.0	0.093	
ICB1	-0.552	0.0	0.001	
CCV1	244.401	0.0	0.232	
CCB1	-0.829	0.0	0.001	
PB122231BL	-0.536	0.0	0.001	
K4088-07	-0.866	0.0	0.001	
K4088-07DUP	-0.627	0.0	0.001	
K4089-02	-0.910	0.0	0.001	
K4096-03	-0.915	0.0	0.001	
K4322-01	0.121	0.0	0.002	
K4322-02	-0.713	0.0	0.001	
CCV2	257.234	0.0	0.245	
CCB2	-0.501	0.0	0.001	

N	13
Mean	45.503
SD	94.9781
CV%	208.73

Aquakem v. 7.2AQ1

Results from time period:

Wed Aug 14 09:33:47 2019

Wed Aug 14 12:01:30 2019

CT

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.4428	µg/l	8/14/2019 9:33:47	
5.0PPBCN	A	Reactive CN	P	4.1344	µg/l	8/14/2019 9:33:48	
10PPBCN	A	Reactive CN	P	8.9764	µg/l	8/14/2019 9:33:49	
50PPBCN	A	Reactive CN	P	49.3379	µg/l	8/14/2019 9:33:50	
100PPBCN	A	Reactive CN	P	100.5278	µg/l	8/14/2019 9:33:51	
250PPBCN	A	Reactive CN	P	253.1819	µg/l	8/14/2019 9:33:52	
500PPBCN	A	Reactive CN	P	498.3988	µg/l	8/14/2019 9:33:53	
ICV1	S	Reactive CN	P	96.2345	µg/l	8/14/2019 11:58:06	
ICB1	S	Reactive CN	P	-0.5519	µg/l	8/14/2019 11:58:07	
CCV1	S	Reactive CN	P	244.4013	µg/l	8/14/2019 11:58:08	
CCB1	S	Reactive CN	P	-0.8295	µg/l	8/14/2019 11:58:09	
PB122231BL	S	Reactive CN	P	-0.5357	µg/l	8/14/2019 11:58:10	
K4088-07	S	Reactive CN	P	-0.8655	µg/l	8/14/2019 11:58:11	
K4088-07DUP	S	Reactive CN	P	-0.6266	µg/l	8/14/2019 11:58:12	
K4089-02	S	Reactive CN	P	-0.9096	µg/l	8/14/2019 11:58:13	
K4096-03	S	Reactive CN	P	-0.9147	µg/l	8/14/2019 11:58:14	
K4322-01	S	Reactive CN	P	0.1214	µg/l	8/14/2019 11:58:15	
K4322-02	S	Reactive CN	P	-0.7131	µg/l	8/14/2019 11:58:16	
CCV2	S	Reactive CN	P	257.2343	µg/l	8/14/2019 12:01:29	
CCB2	S	Reactive CN	P	-0.5013	µg/l	8/14/2019 12:01:30	