

UB105254

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/20/2019 11:51

Test: ~~Total~~ CN

Reactive
ug/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.500	0.0	0.094	
ICB1	0.906	0.0	0.002	
CCV1	240.149	0.0	0.227	
CCB1	1.065	0.0	0.002	
PB123236BL	0.853	0.0	0.002	
K4662-15	1.031	0.0	0.002	
K4662-15DUP	0.717	0.0	0.002	
K4957-13	0.751	0.0	0.002	
K4957-14	0.770	0.0	0.002	
K4957-15	0.757	0.0	0.002	
K4957-16	0.629	0.0	0.002	
K4957-17	0.842	0.0	0.002	
K4957-18	0.910	0.0	0.002	
CCV2	251.339	0.0	0.237	
CCB2	0.768	0.0	0.002	

N 15
Mean 39.999
SD 87.2414
CV% 218.11

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/20/2019 11:33

Test

Reactive
~~Total~~ CN

Accepted

9/20/2019 8:42

Factor

1064


Bias

0.001

Coeff. of det.

0.998950

Errors

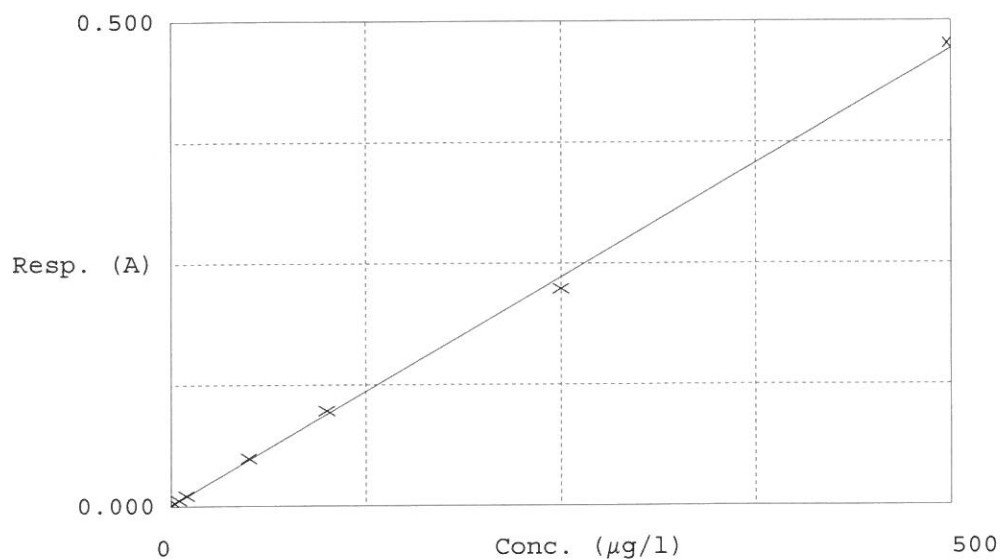

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.6653	0.0000	
2	5.0PPBCN	0.006	5.7959	5.0000	
3	10PPBCN	0.011	10.8886	10.0000	
4	50PPBCN	0.049	51.4056	50.0000	
5	100PPBCN	0.098	103.6132	100.0000	
6	250PPBCN	0.224	237.0406	250.0000	
7	500PPBCN	0.476	505.5907	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri Sep 20 11:42:14 2019

Fri Sep 20 11:46:36 2019

CT
9/20/19

Sample Id	Sam/Ctr/c	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	ReactiveCN	P	0.6653	µg/l	9/20/2019 8:40:41	
5.0PPBCN	A	ReactiveCN	P	5.7959	µg/l	9/20/2019 8:40:42	
10PPBCN	A	ReactiveCN	P	10.8886	µg/l	9/20/2019 8:40:43	
50PPBCN	A	ReactiveCN	P	51.4056	µg/l	9/20/2019 8:40:44	
100PPBCN	A	ReactiveCN	P	103.6132	µg/l	9/20/2019 8:40:45	
250PPBCN	A	ReactiveCN	P	237.0406	µg/l	9/20/2019 8:40:46	
500PPBCN	A	ReactiveCN	P	505.5907	µg/l	9/20/2019 8:40:47	
ICV1	S	ReactiveCN	P	98.4997	µg/l	9/20/2019 11:42:14	
ICB1	S	ReactiveCN	P	0.9057	µg/l	9/20/2019 11:42:15	
CCV1	S	ReactiveCN	P	240.1492	µg/l	9/20/2019 11:42:16	
CCB1	S	ReactiveCN	P	1.0648	µg/l	9/20/2019 11:42:17	
PB123236BL	S	ReactiveCN	P	0.8529	µg/l	9/20/2019 11:42:18	
K4662-15	S	ReactiveCN	P	1.0314	µg/l	9/20/2019 11:42:19	
K4662-15DUP	S	ReactiveCN	P	0.7167	µg/l	9/20/2019 11:42:20	
K4957-13	S	ReactiveCN	P	0.7513	µg/l	9/20/2019 11:42:21	
K4957-14	S	ReactiveCN	P	0.7702	µg/l	9/20/2019 11:42:22	
K4957-15	S	ReactiveCN	P	0.7575	µg/l	9/20/2019 11:42:23	
K4957-16	S	ReactiveCN	P	0.6295	µg/l	9/20/2019 11:42:24	
K4957-17	S	ReactiveCN	P	0.8421	µg/l	9/20/2019 11:46:33	
K4957-18	S	ReactiveCN	P	0.9102	µg/l	9/20/2019 11:46:34	
CCV2	S	ReactiveCN	P	251.3395	µg/l	9/20/2019 11:46:35	
CCB2	S	ReactiveCN	P	0.7679	µg/l	9/20/2019 11:46:36	