

LB105334

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/26/2019 12:31

Test: ~~Total~~ ^{Reactive} CN

al26/19
OT

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	92.714	0.0	0.079	
ICB1	1.349	0.0	0.002	
CCV1	237.272	0.0	0.201	
CCB1	0.945	0.0	0.002	
PB123374BL	1.048	0.0	0.002	
K4657-03DUP	0.730	0.0	0.001	
K4657-06	0.767	0.0	0.001	
K4663-09	0.398	0.0	0.001	
K5012-01	0.906	0.0	0.001	
K4657-03	1.248	0.0	0.002	
CCV2	256.437	0.0	0.217	
CCB2	1.234	0.0	0.002	

N 12
Mean 49.587
SD 95.8958
CV% 193.39

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/26/2019 8:23


Test ~~Total~~ ^{Reactive} CN

Accepted 9/26/2019 8:23

Factor 1185
Bias 0.001

Coeff. of det. 0.999969

Errors

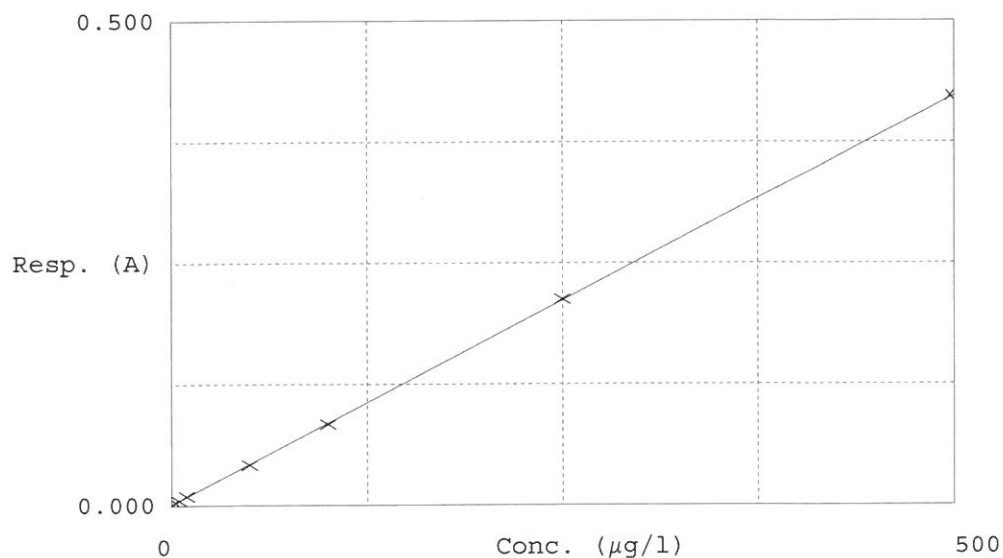

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.8179	0.0000	
2	5.0PPBCN	0.005	5.3286	5.0000	
3	10PPBCN	0.010	10.6226	10.0000	
4	50PPBCN	0.042	48.9125	50.0000	
5	100PPBCN	0.084	98.3458	100.0000	
6	250PPBCN	0.213	251.0975	250.0000	
7	500PPBCN	0.422	499.8751	500.0000	

9/26/19

CT

Aquakem v. 7.2AQ1

Results from time period:

Thu Sep 26 11:53:36 2019

Thu Sep 26 12:30:16 2019

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.8179	µg/l	9/26/2019 8:17:45	
5.0PPBCN	A	Reactive CN	P	5.3286	µg/l	9/26/2019 8:17:46	
10PPBCN	A	Reactive CN	P	10.6226	µg/l	9/26/2019 8:17:47	
50PPBCN	A	Reactive CN	P	48.9125	µg/l	9/26/2019 8:17:48	
100PPBCN	A	Reactive CN	P	98.3458	µg/l	9/26/2019 8:17:49	
250PPBCN	A	Reactive CN	P	251.0975	µg/l	9/26/2019 8:17:50	
500PPBCN	A	Reactive CN	P	499.8751	µg/l	9/26/2019 8:17:51	
ICV1	S	Reactive CN	P	92.7143	µg/l	9/26/2019 11:53:36	
ICB1	S	Reactive CN	P	1.3489	µg/l	9/26/2019 11:53:37	
CCV1	S	Reactive CN	P	237.272	µg/l	9/26/2019 11:53:38	
CCB1	S	Reactive CN	P	0.9447	µg/l	9/26/2019 11:53:39	
PB123374BL	S	Reactive CN	P	1.0485	µg/l	9/26/2019 11:53:40	
K4657-03DUP	S	Reactive CN	P	0.7298	µg/l	9/26/2019 11:53:42	
K4657-06	S	Reactive CN	P	0.7668	µg/l	9/26/2019 11:53:43	
K4663-09	S	Reactive CN	P	0.3983	µg/l	9/26/2019 11:53:44	
K5012-01	S	Reactive CN	P	0.9063	µg/l	9/26/2019 11:53:45	
K4657-03	S	Reactive CN	P	1.2477	µg/l	9/26/2019 12:30:14	
CCV2	S	Reactive CN	P	256.4371	µg/l	9/26/2019 12:30:15	
CCB2	S	Reactive CN	P	1.2336	µg/l	9/26/2019 12:30:16	