

Clear table

FC-2 3000
10-9-19


ident	concentra tion F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-10-01_	10/1/19 11:47		CT/AP
STD2	0.2370	0.3710	0.3770	1.2480	0.3160	0.3260	1.9060	2019-10-01_	10/1/19 12:18		CT/AP
STD3	0.4310	0.6440	0.6470	2.1690	0.5450	1.0010	3.2530	2019-10-01_	10/1/19 12:49		CT/AP
STD4	0.8150	1.2060	1.2010	4.0210	1.0100	2.1860	6.0250	2019-10-01_	10/1/19 13:20		CT/AP
STD5	1.9150	2.8590	2.8480	9.4780	2.3580	5.0660	14.1850	2019-10-01_	10/1/19 13:51		CT/AP
STD6	3.9010	5.8910	5.9030	19.6450	4.9000	9.8870	29.4500	2019-10-01_	10/1/19 14:22		CT/AP
STD7	5.1010	7.6290	7.6240	25.4390	6.3710	12.5350	38.1810	2019-10-01_	10/1/19 14:53		CT/AP
ICV	2.0230	2.9740	2.9490	9.8290	2.4750	5.3960	15.0740	2019-10-01_	10/1/19 15:27		CT/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-10-01_	10/1/19 16:02		CT/AP
CCV	2.0790	2.9460	2.9340	9.7400	2.4320	5.7170	14.2870	2019-10-08_	10/8/19 10:25		CT/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-10-08_	10/8/19 10:56		CT/AP
LB105569BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-10-08_	10/8/19 11:27		CT/AP
LB105569BSW	2.0470	2.9490	2.9350	9.7190	2.4300	5.9470	14.3240	2019-10-08_	10/8/19 11:58		CT/AP
K5260-02	0.0000	47.4110	0.0000	0.0000	0.3490	2.8400	30.1230	2019-10-08_	10/8/19 14:19		CT/AP
K5260-03	0.0000	40.1800	0.0000	0.0000	0.3890	0.0000	29.5520	2019-10-08_	10/8/19 14:49		CT/AP
K5260-06	0.0000	54.1330	0.0000	0.0000	0.3780	0.0000	26.7620	2019-10-08_	10/8/19 15:20		CT/AP
K5260-07	0.0000	38.1860	0.0000	0.0000	0.3850	0.0000	29.0710	2019-10-08_	10/8/19 15:51		CT/AP
K5260-08	0.0000	38.1590	0.0000	0.0000	0.3860	0.0000	29.0570	2019-10-08_	10/8/19 16:22		CT/AP
K5260-09	0.0000	48.9020	0.0000	0.0000	0.3650	0.0000	27.3520	2019-10-08_	10/8/19 16:53		CT/AP
K5260-10	0.0000	8.4220	0.3120	0.0000	0.0000	0.0000	1.6250	2019-10-08_	10/8/19 17:24		CT/AP
K5260-11	0.0000	11.6810	0.0000	0.0000	0.1400	0.0000	26.0800	2019-10-08_	10/8/19 17:55		CT/AP
CCV	1.9310	2.8860	2.8430	9.5770	2.3840	5.9980	13.7910	2019-10-08_	10/8/19 18:26		CT/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-10-08_	10/8/19 18:57		CT/AP
K5260-12	0.0000	13.9380	0.0000	0.0000	0.4230	0.0000	29.7400	2019-10-08_	10/8/19 19:29		CT/AP
K5260-13	0.0000	13.0380	0.0000	0.0000	0.4150	0.0000	27.3390	2019-10-08_	10/8/19 20:00		CT/AP
K5260-03DUP	0.0000	40.5310	0.0000	0.0000	0.3960	0.0000	29.7810	2019-10-08_	10/8/19 20:31		CT/AP
K5260-04MS	2.3520	39.9500	2.8620	10.2130	2.8810	9.9710	42.9190	2019-10-08_	10/8/19 21:02		CT/AP
K5260-05MSD	2.3060	39.9760	2.8650	10.1840	2.8630	9.9770	42.8640	2019-10-08_	10/8/19 21:33		CT/AP
CCV	1.9370	2.9090	2.8370	9.5890	2.3890	5.8910	13.5920	2019-10-08_	10/8/19 22:04		CT/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-10-08_	10/8/19 22:35		CT/AP

CALIBRATION OF COMPONENT F-

IC-2

Method: AnionsIC2-100119.mtw
 Equation: $Q = 0.0168603 \cdot A + 1.59581$
 RSD: 4.181 %
 Correlation coefficient: 0.999261

10-

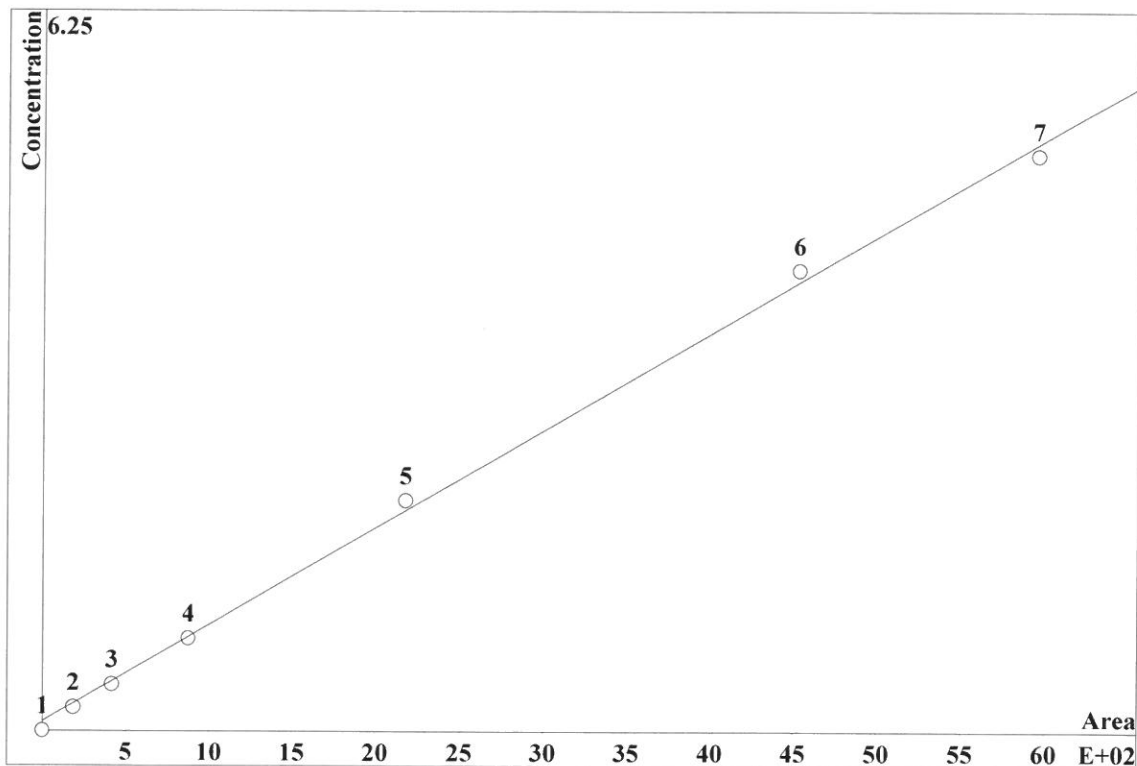


K3 = 0 K2 = 0 K1 = 0.0168603 K0 = 1.59581
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1		0	0	0		0
2	5.217	186.5	0.2		20	
3	11.15	416.3	0.4		20	
4	25.52	872.7	0.8		20	
5	62.75	2177	2		20	
6	130.1	4532	4		20	
7	180	5956	5		20	

000

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-100119.mtw
 Equation: $Q = 0.0243407 \cdot A + 2.12645$
 RSD: 3.796 %
 Correlation coefficient: 0.999391

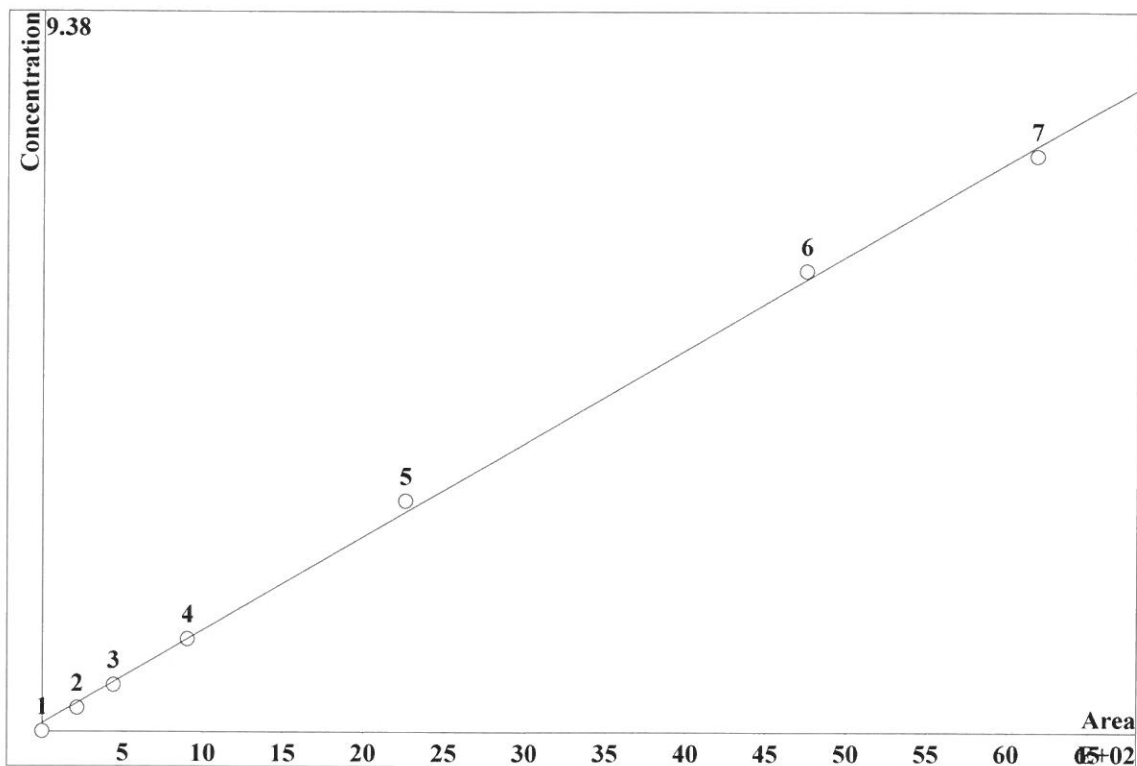


K3 = 0 K2 = 0 K1 = 0.0243407 K0 = 2.12645
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1		0	0	0		0
2	13.31	217.4	0.3		20	
3	27.32	442	0.6		20	
4	55.74	903.8	1.2		20	
5	140	2261	3		20	
6	299.3	4753	6		20	
7	392.2	6181	7.5		20	

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-100119.mtw
Equation: $Q = 0.0105965 \cdot A + 2.67926$
RSD: 3.819 %
Correlation coefficient: 0.999383

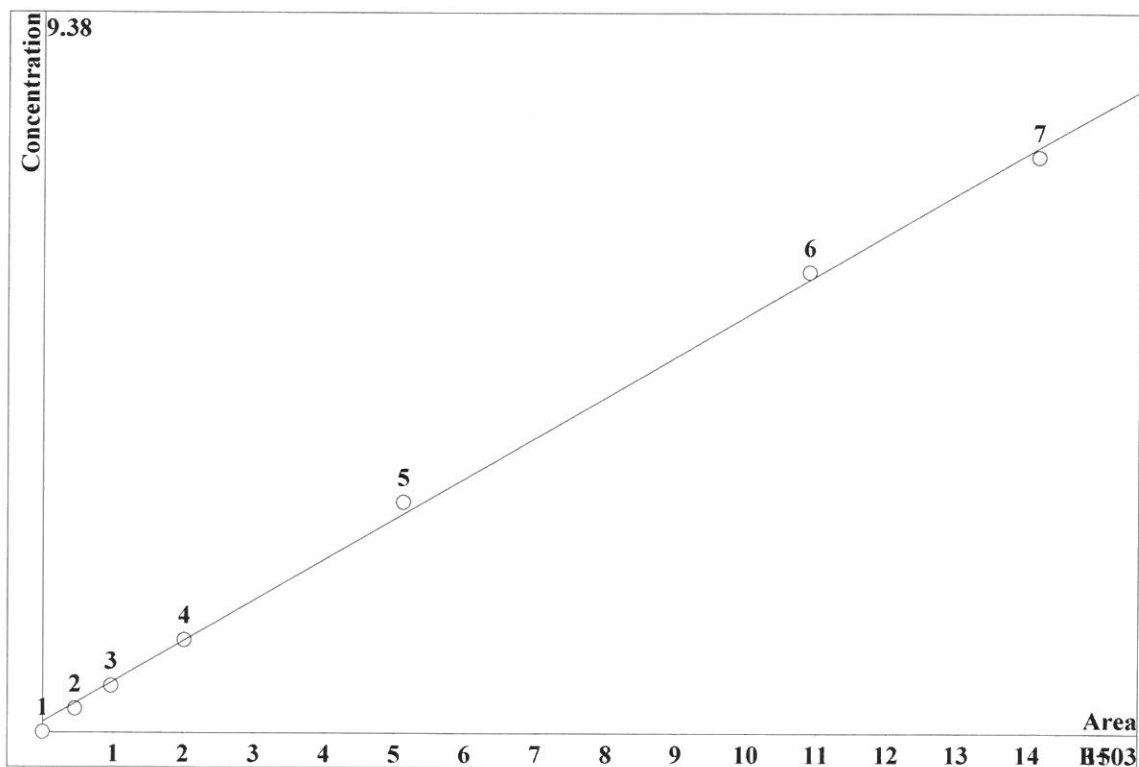


K3 = 0 K2 = 0 K1 = 0.0105965 K0 = 2.67926
Base: Area
Ref.channel: chl
ISTD:
Formula: Linear
Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	22.83	458.8	0.3	20			
3	48.33	967.9	0.6	20			
4	99.37	2014	1.2	20			
5	249.6	5123	3	20			
6	514.2	1.089e+04	6	20			
7	650.9	1.414e+04	7.5	20			

5?&

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-100119.mtw
 Equation: $Q = 0.0542276 \cdot A + 7.84878$
 RSD: 3.997 %
 Correlation coefficient: 0.999325

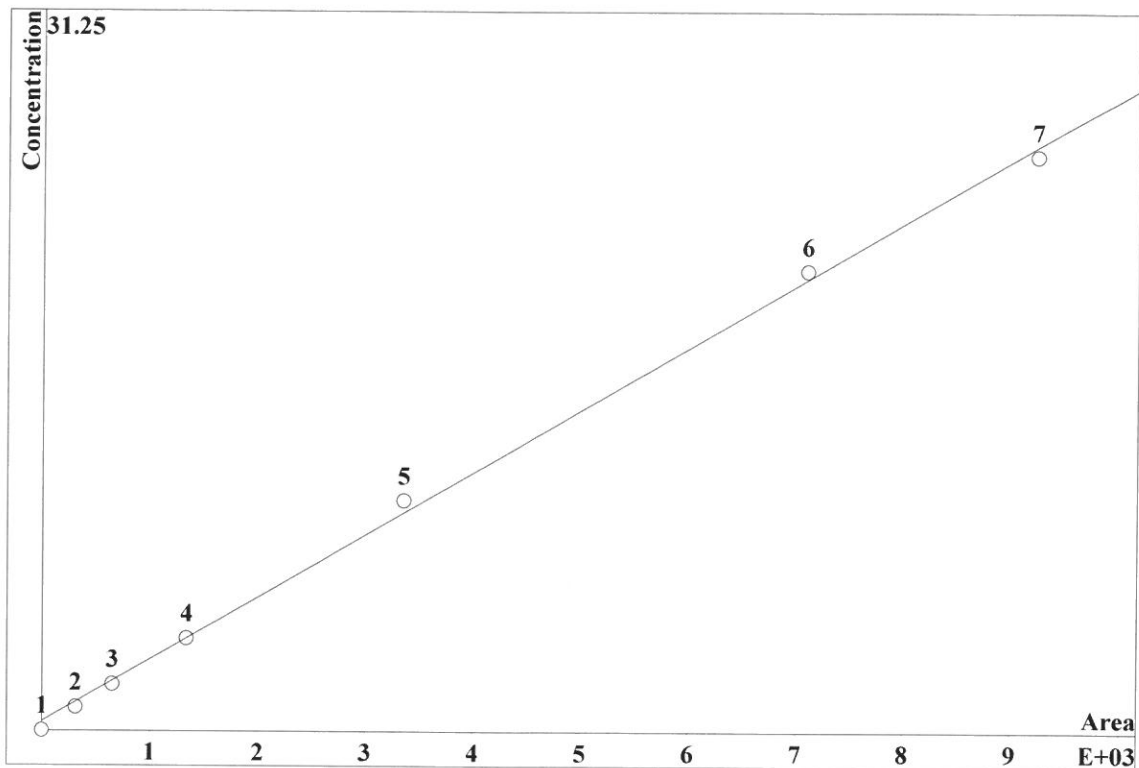


K3 = 0 K2 = 0 K1 = 0.0542276 K0 = 7.84878
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	
2	14.04	315.7	1	20		
3	29.21	655.4	2	20		
4	60.29	1338	4	20		
5	153.6	3351	10	20		
6	334.7	7101	20	20		
7	439.4	9238	25	20		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-100119.mtw
 Equation: $Q = 0.00958397 \cdot A + 2.05722$
 RSD: 4.381 %
 Correlation coefficient: 0.999189

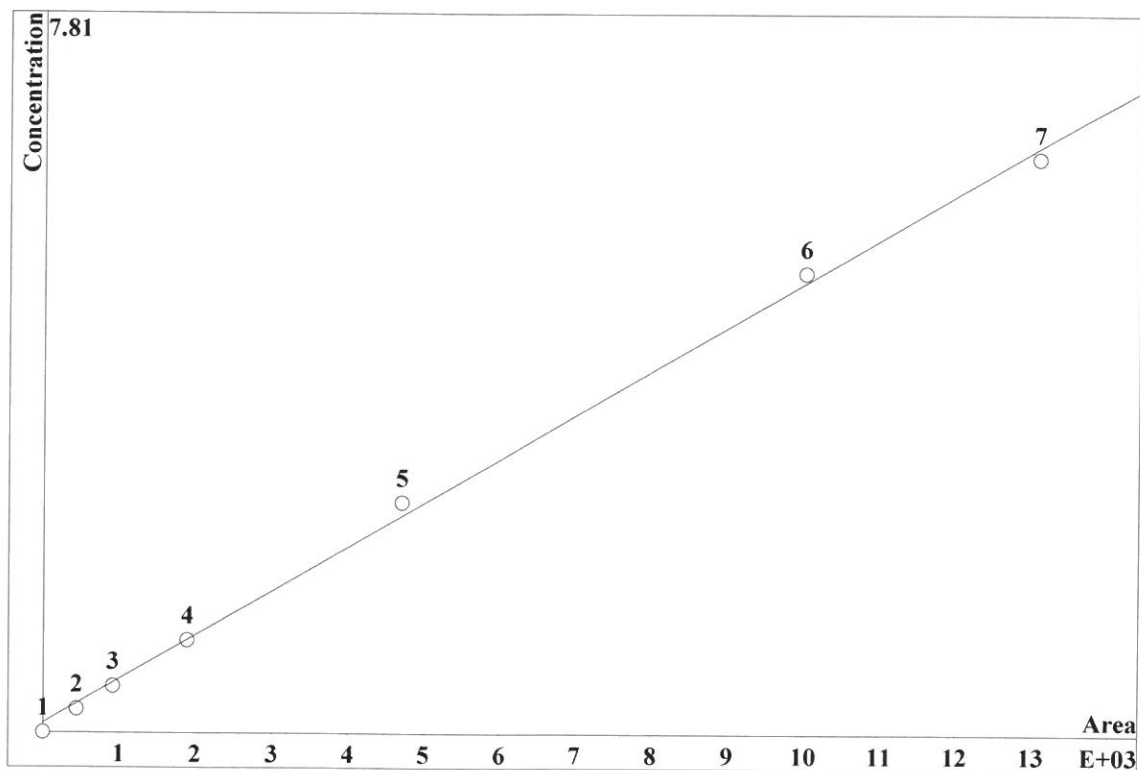


K3 = 0 K2 = 0 K1 = 0.00958397 K0 = 2.05722
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1		0	0		0		0
2	16.28		445.2	0.25			20
3	34.07		922.7	0.5			20
4	70.26		1893	1			20
5	177.5		4706	2.5			20
6	387.2	1.001e+04		5			20
7	511.7	1.308e+04		6.25			20

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-100119.mtw
Equation: $Q = 0.0208939 \cdot A - 4.09382$
RSD: 2.789 %
Correlation coefficient: 0.999671

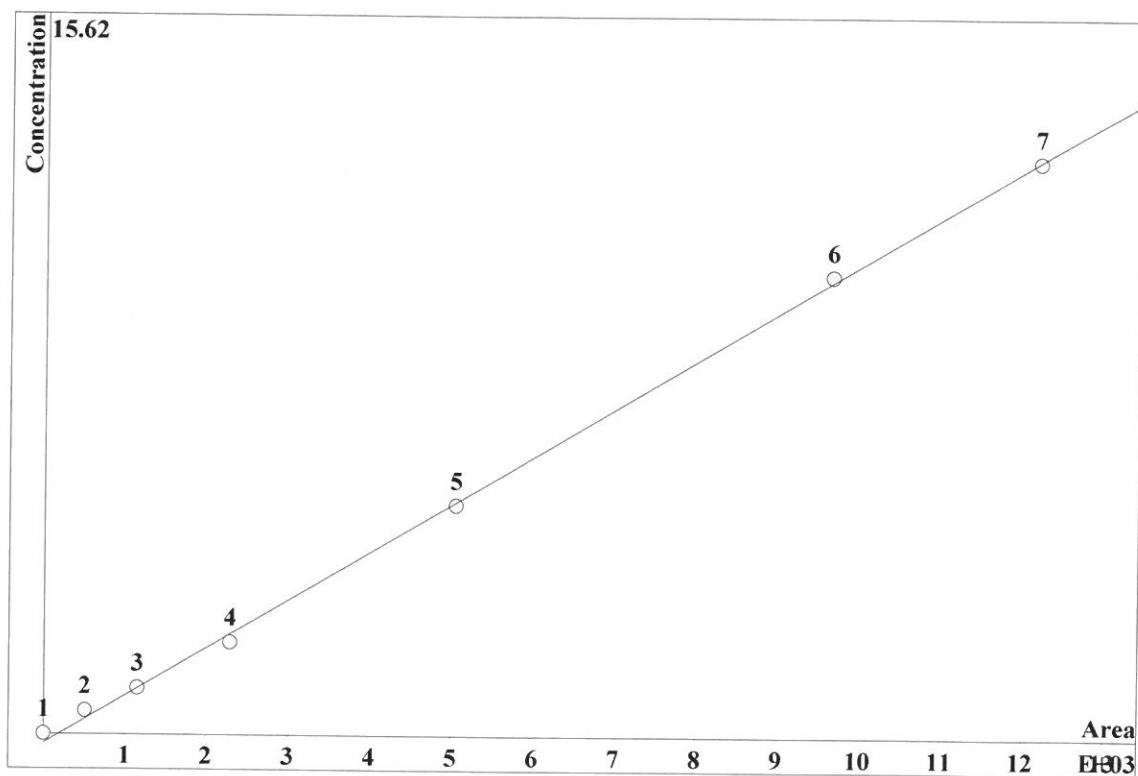


K3 = 0 K2 = 0 K1 = 0.0208939 K0 = -4.09382
Base: Area
Ref.channel: ch1
ISTD:
Formula: Linear
Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	10.86	508.3	0.5	20			
3	25	1154	1	20			
4	51.74	2288	2	20			
5	119.7	5045	5	20			
6	238.5	9660	10	20			
7	306.5	1.219e+04	12.5	20			

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-100119.mtw
 Equation: $Q = 0.0322739 \cdot A + 9.52592$
 RSD: 4.157 %
 Correlation coefficient: 0.999269

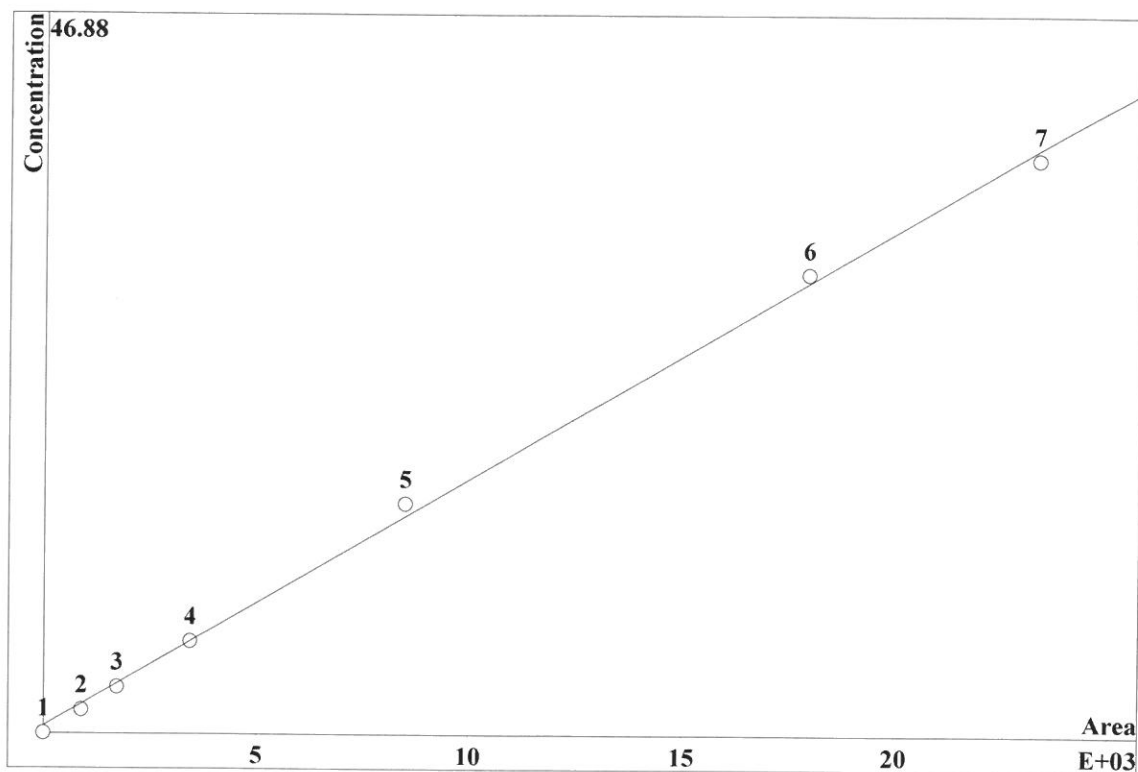

K3 = 0 K2 = 0 K1 = 0.0322739 K0 = 9.52592
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	22.09	886	1.5	20			
3	43.59	1721	3	20			
4	87.87	3439	6	20			
5	220	8495	15	20			
6	469	1.795e+04	30	20			
7	610.5	2.337e+04	37.5	20			

Report date: 10/7/2019 3:43:47 PM
Printed by: wet


Ident: STD1
Analysis from: 10/1/2019 11:47:17 AM
File: _2019-10-01_

Last save: 10/1/2019 3:23:

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22632

Last save: 10/1/20

SAMPLE:
: CT/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

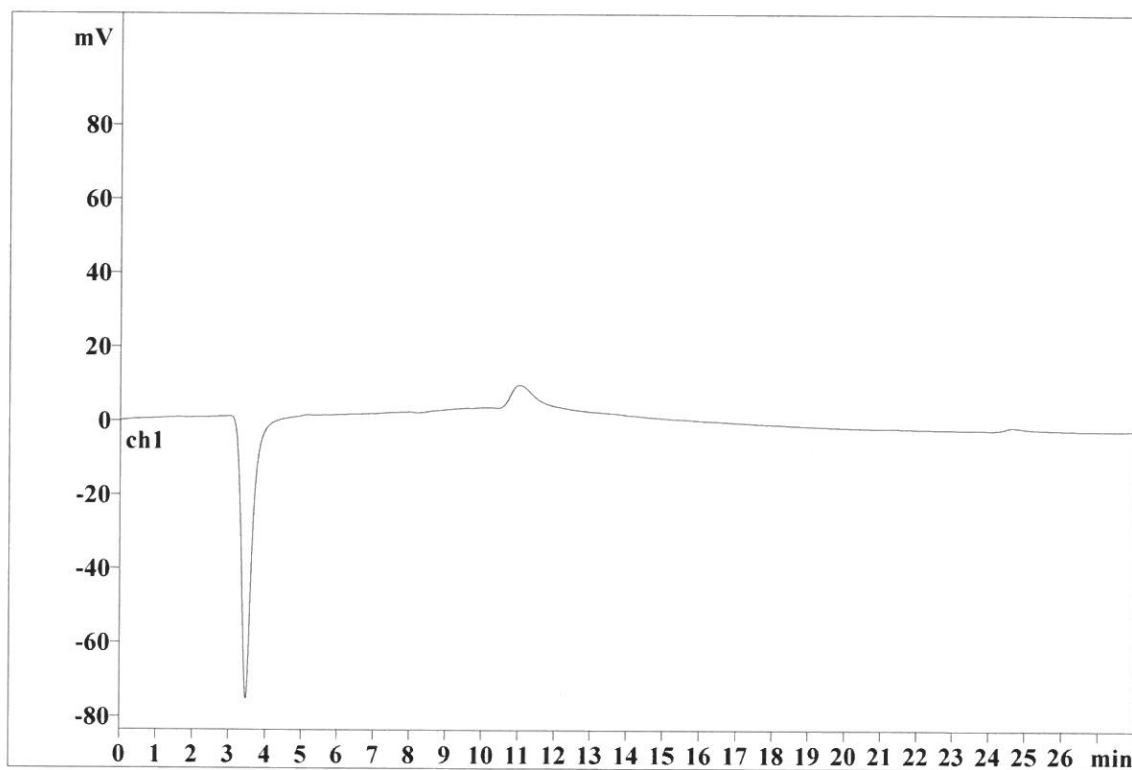

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/7/2019 3:43:57 PM
Printed by: wet


Ident: STD2
Analysis from: 10/1/2019 12:18:16 PM
File: _2019-10-01_

Last save: 10/1/2019 3:23:

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22633

Last save: 10/1/20

SAMPLE:
: CT/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

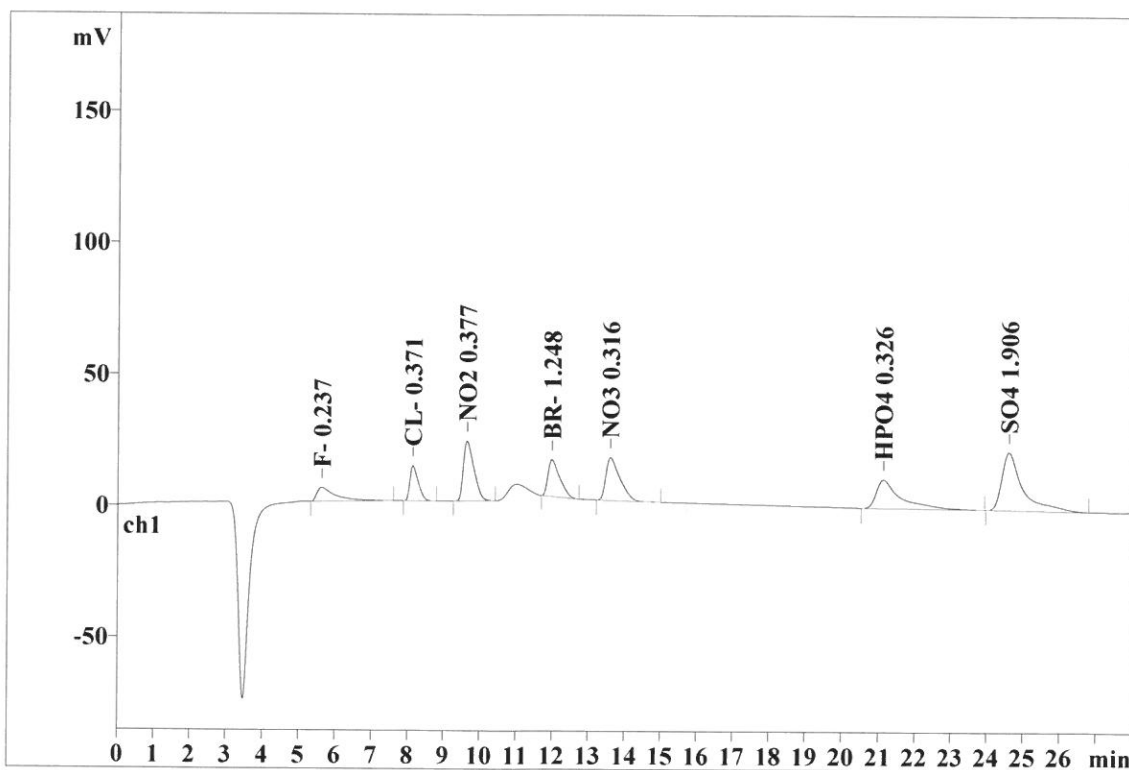

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec
1	5.62	0.468	5.22	4.99	186.541
2	8.12	0.255	13.31	12.72	217.377
3	9.62	0.315	22.82	21.81	458.778
4	11.97	0.348	14.04	13.42	315.664
5	13.59	0.424	16.28	15.56	445.202
6	21.12	0.561	10.85	10.37	508.257
7	24.60	0.507	22.09	21.11	885.981
7	28.00	0.411	104.62	99.99	3017.800

This report has been created by IC Net
METROHM LTD

Report date: 10/7/2019 3:44:07 PM
Printed by: wet


Ident: STD3
Analysis from: 10/1/2019 12:49:14 PM
File: _2019-10-01_

Last save: 10/1/2019 3:23:

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22634

Last save: 10/1/20

SAMPLE:
: CT/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

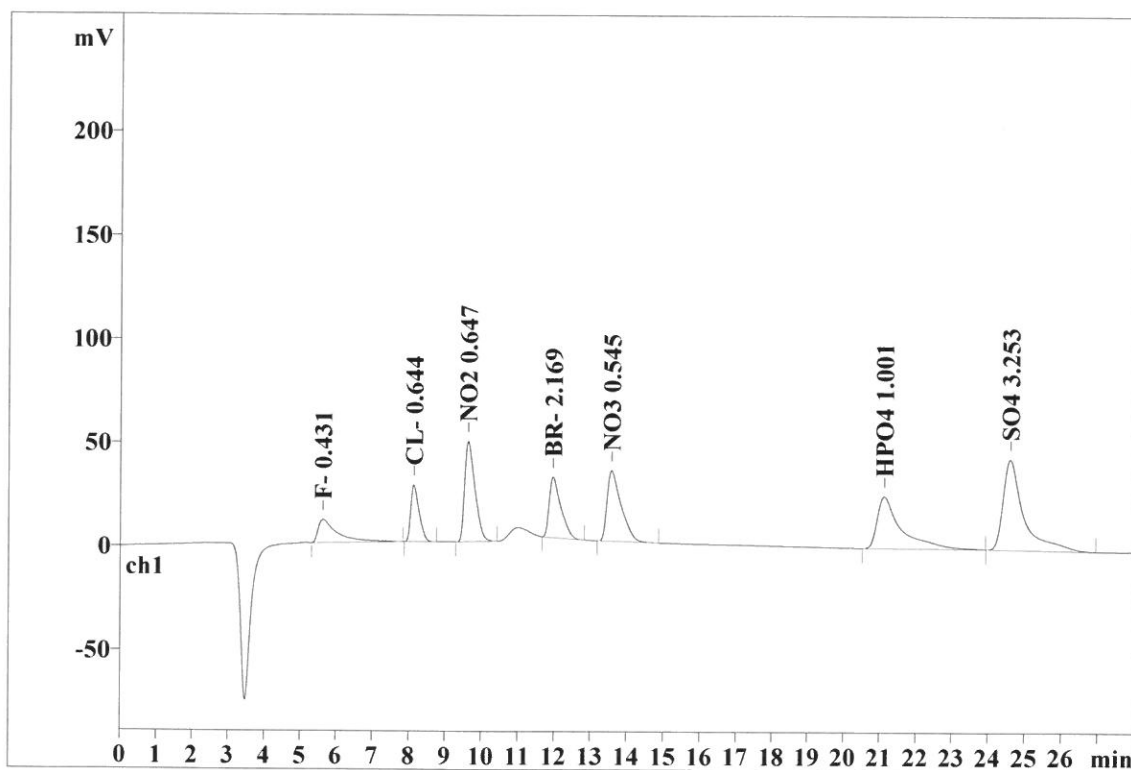

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec
1	5.63	0.479	11.14	5.10	416.290
2	8.12	0.251	27.32	12.50	441.974
3	9.61	0.312	48.33	22.10	967.889
4	11.96	0.340	29.21	13.36	655.386
5	13.57	0.413	34.07	15.58	922.664
6	21.11	0.549	24.99	11.43	1153.705
7	24.59	0.498	43.59	19.93	1720.614
7	28.00	0.406	218.65	100.00	6278.521

This report has been created by IC Net
METROHM LTD

Report date: 10/7/2019 3:44:18 PM
Printed by: wet


Ident: STD4
Analysis from: 10/1/2019 1:20:14 PM
File: _2019-10-01_

Last save: 10/1/2019 3:23

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22635

Last save: 10/1/2019 3:23

SAMPLE:
: CT/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

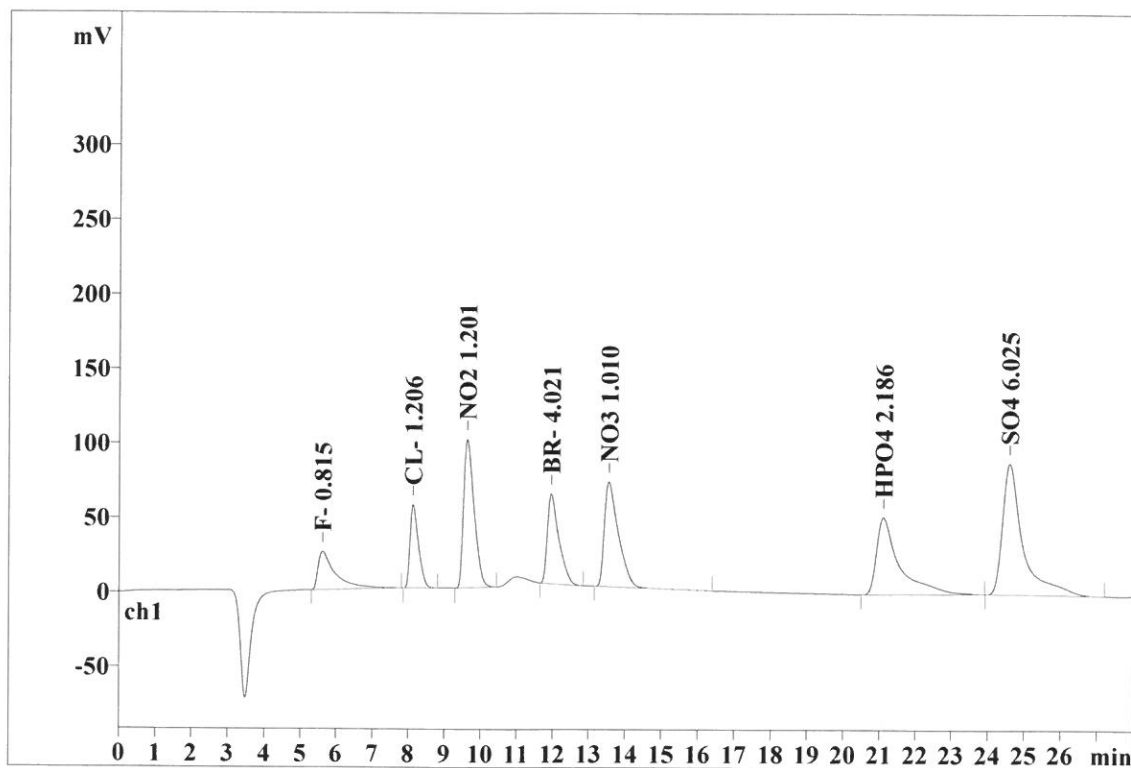

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec
1	5.61	0.437	25.52	5.66	872.665
2	8.12	0.249	55.73	12.36	903.761
3	9.61	0.315	99.37	22.04	2014.426
4	11.94	0.332	60.29	13.37	1338.145
5	13.54	0.405	70.26	15.59	1892.987
6	21.10	0.525	51.74	11.48	2288.201
7	24.59	0.494	87.87	19.49	3438.579
7	28.00	0.394	450.78	100.00	12748.764

This report has been created by IC Net
METROHM LTD

Report date: 10/7/2019 3:44:27 PM
Printed by: wet


Ident: STD5
Analysis from: 10/1/2019 1:51:13 PM
File: _2019-10-01_

Last save: 10/1/2019 3:23

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22636

Last save: 10/1/2019

SAMPLE:
: CT/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

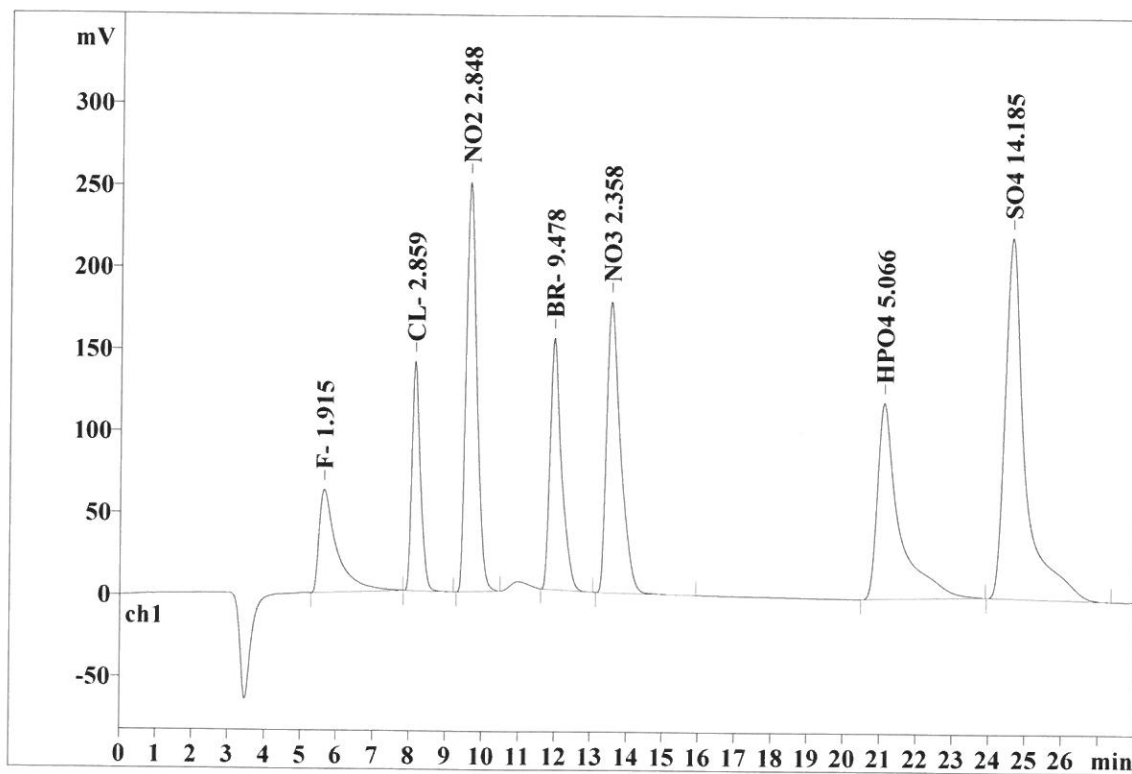

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec
1	5.63	0.459	62.75	5.59	2176.991
2	8.12	0.244	140.02	12.47	2261.454
3	9.60	0.317	249.62	22.22	5122.872
4	11.94	0.319	153.55	13.67	3350.828
5	13.52	0.395	177.46	15.80	4706.320
6	21.09	0.503	119.66	10.65	5045.007
7	24.58	0.488	220.04	19.59	8495.077
7	28.00	0.389	1123.11	100.00	31158.548

Report date: 10/7/2019 3:44:36 PM
Printed by: wet


Ident: STD6
Analysis from: 10/1/2019 2:22:11 PM
File: _2019-10-01_

Last save: 10/1/2019 3:23:

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22637

Last save: 10/1/20

SAMPLE:
: CT/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

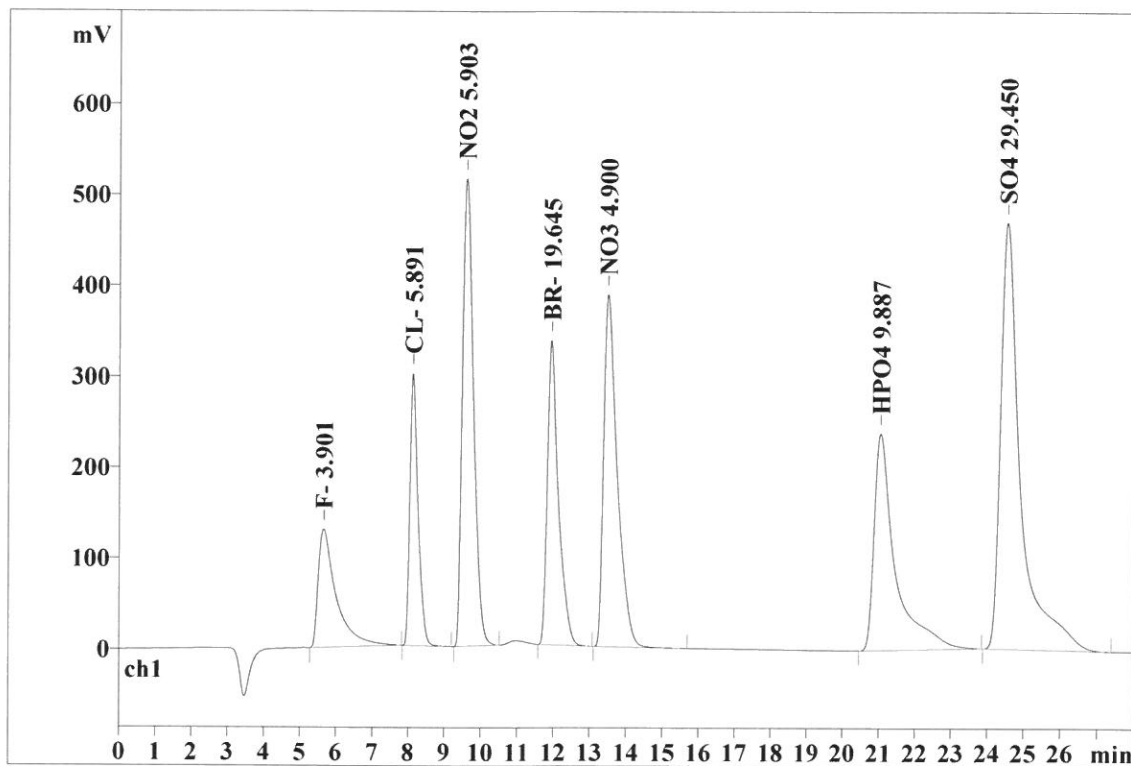

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec
1	5.65	0.469	130.08	5.48	4532.376
2	8.11	0.238	299.25	12.61	4753.405
3	9.58	0.329	514.18	21.67	10887.895
4	11.93	0.304	334.64	14.10	7100.605
5	13.49	0.380	387.13	16.32	10010.635
6	21.04	0.490	238.54	10.05	9659.749
7	24.54	0.488	468.99	19.76	17954.862
7	28.00	0.385	2372.81	100.00	64899.526

This report has been created by IC Net
METROHM LTD

Report date: 10/7/2019 3:44:44 PM
Printed by: wet


Ident: STD7
Analysis from: 10/1/2019 2:53:10 PM
File: _2019-10-01_

Last save: 10/1/2019 3:23:

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22638

Last save: 10/1/20

SAMPLE:
: CT/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

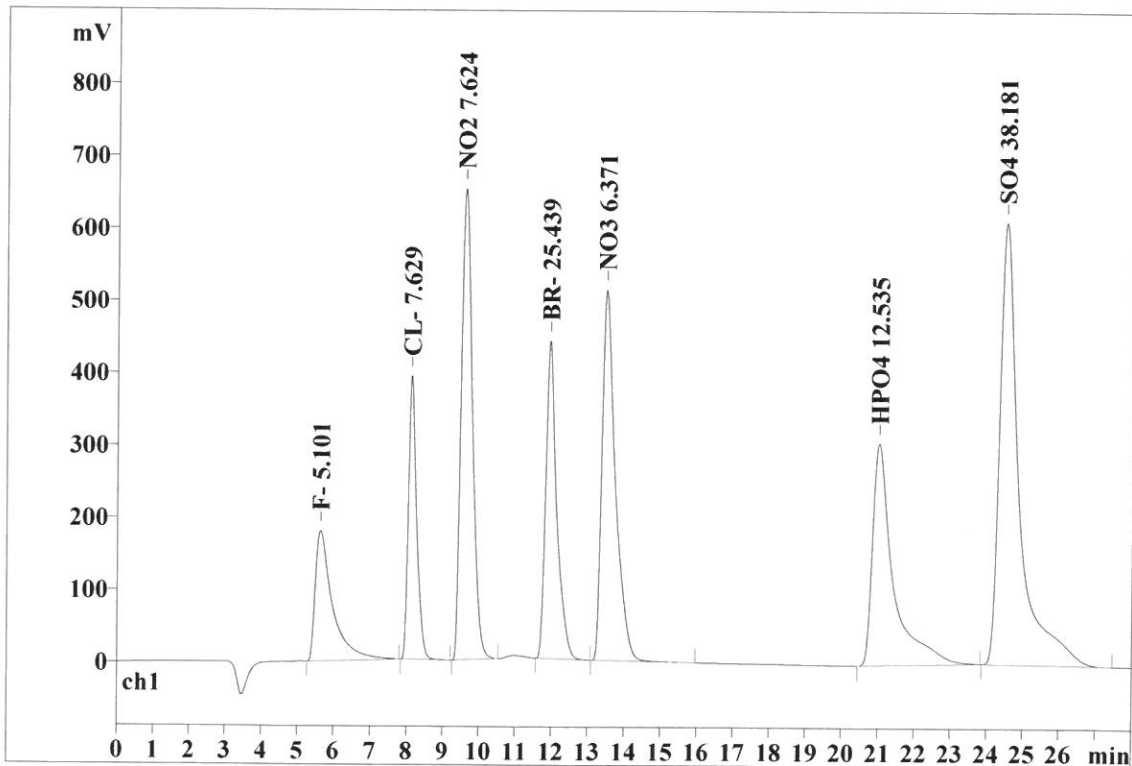

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec
1	5.63	0.442	180.02	5.82	5956.337
2	8.11	0.234	392.21	12.69	6180.922
3	9.57	0.338	650.91	21.06	14137.076
4	11.93	0.298	439.42	14.21	9237.529
5	13.48	0.372	511.70	16.55	13079.948
6	21.02	0.485	306.50	9.91	12194.476
7	24.52	0.489	610.46	19.75	23365.712
7	28.00	0.380	3091.23	100.00	84152.000

Report date: 10/7/2019 3:44:56 PM
Printed by: wet


Ident: ICV
Analysis from: 10/1/2019 3:27:08 PM
File: _2019-10-01_

Last save: 10/1/2019 3:55

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22639

Last save: 10/1/2019 3:55

SAMPLE:
: CT/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

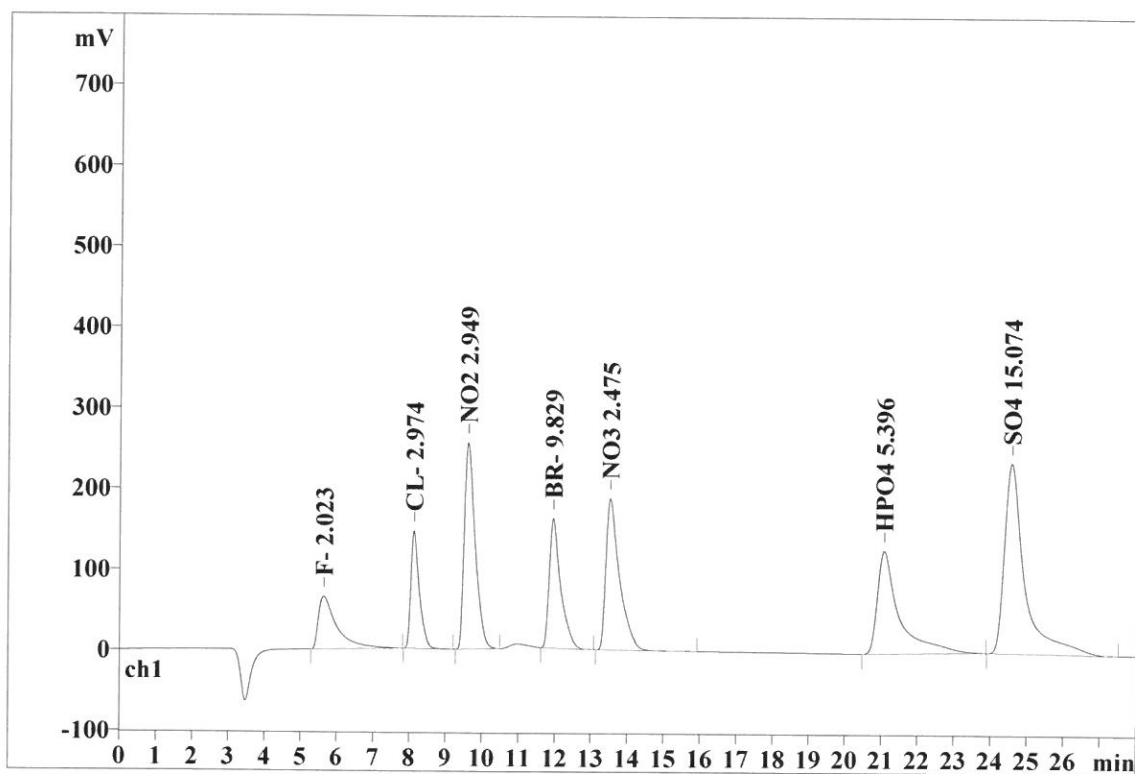

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec
1	5.63	0.471	65.11	5.54	2304.605
2	8.11	0.240	145.50	12.37	2355.990
3	9.59	0.317	255.18	21.70	5312.747
4	11.94	0.309	160.27	13.63	3480.214
5	13.51	0.383	187.36	15.93	4951.250
6	21.07	0.499	127.32	10.83	5361.438
7	24.56	0.484	235.08	19.99	9046.134
7	28.00	0.386	1175.81	100.00	32812.379

This report has been created by IC Net
METROHM LTD

Report date: 10/7/2019 3:45:06 PM
Printed by: wet


Ident: ICB
Analysis from: 10/1/2019 4:02:11 PM
File: _2019-10-01_

Last save: 10/1/2019 4:30

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22640

Last save: 10/1/2019 4:30

SAMPLE:
: CT/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

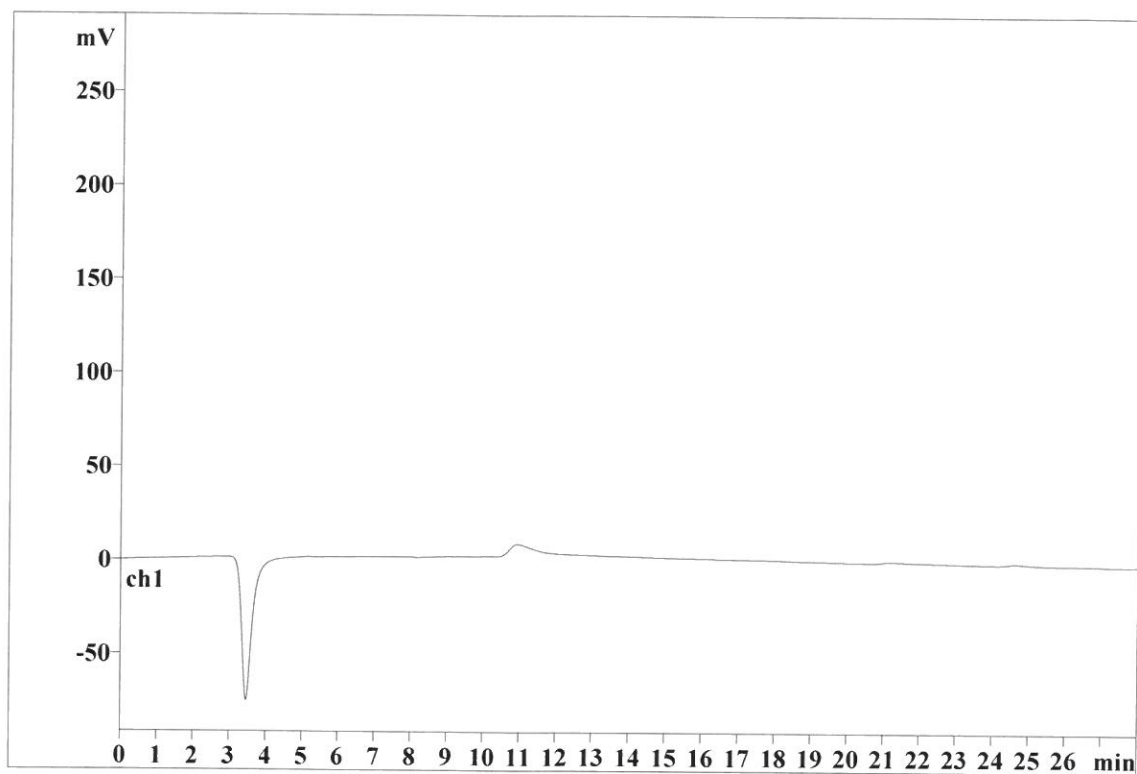

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:20:35 AM

Printed by: wet

Ident: CCV

Analysis from: 10/8/2019 10:25:59 AM

File: _2019-10-08_

Last save: 10/8/2019 10:53:59 AM

Method: AnionsIC2-100119.mtw

Last save: 10/1/2019 3:21:

Run operator: wet

Analysis number: 22709

SAMPLE:


: CT/AP

Vial number: 2

Volume: 20.0 µL

Dilution: 1.00

Amount: 1.0000

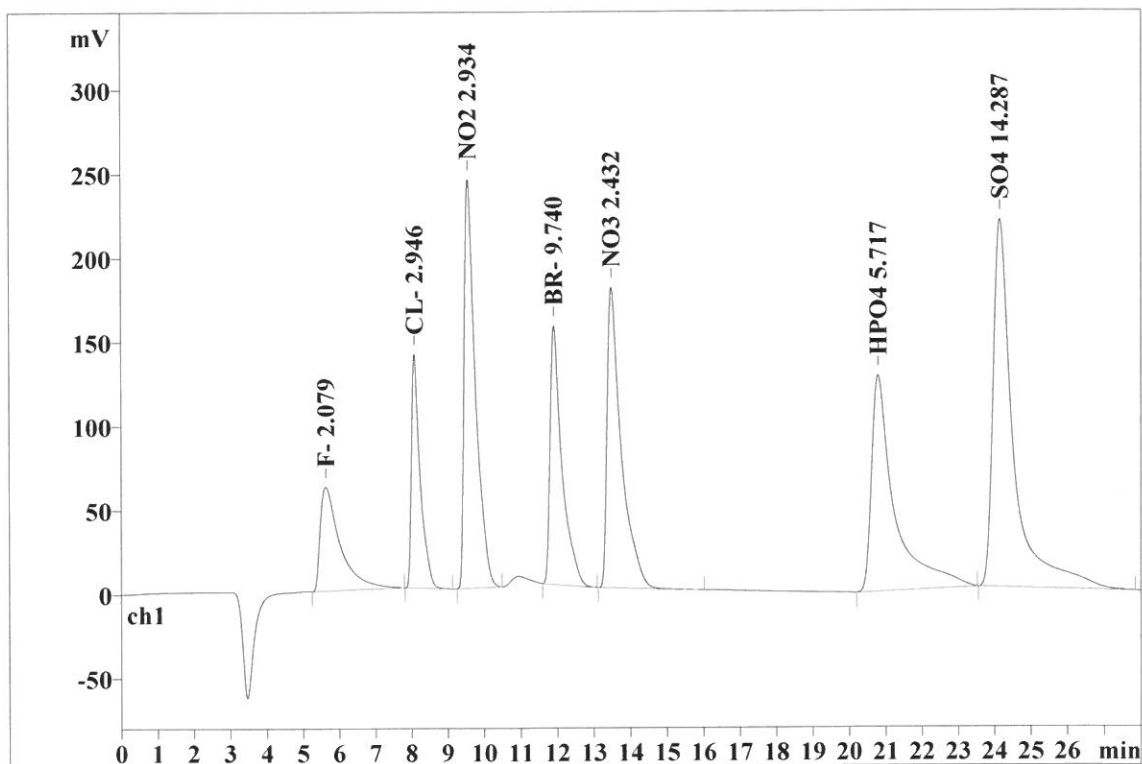

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.525	61.70	5.49	2371.850	7.29
2	8.07	0.238	139.09	12.37	2333.410	7.17
3	9.55	0.319	243.32	21.64	5284.550	16.25
4	11.91	0.305	153.96	13.69	3447.552	10.60
5	13.48	0.376	178.86	15.91	4860.687	14.94
6	20.81	0.517	128.51	11.43	5668.787	17.43
7	24.18	0.488	218.75	19.46	8558.193	26.31
7	28.00	0.395	1124.18	100.00	32525.028	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:20:47 AM
Printed by: wet


Ident: CCB
Analysis from: 10/8/2019 10:56:58 AM
File: _2019-10-08_

Last save: 10/8/2019 11:24:58 AM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22710

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

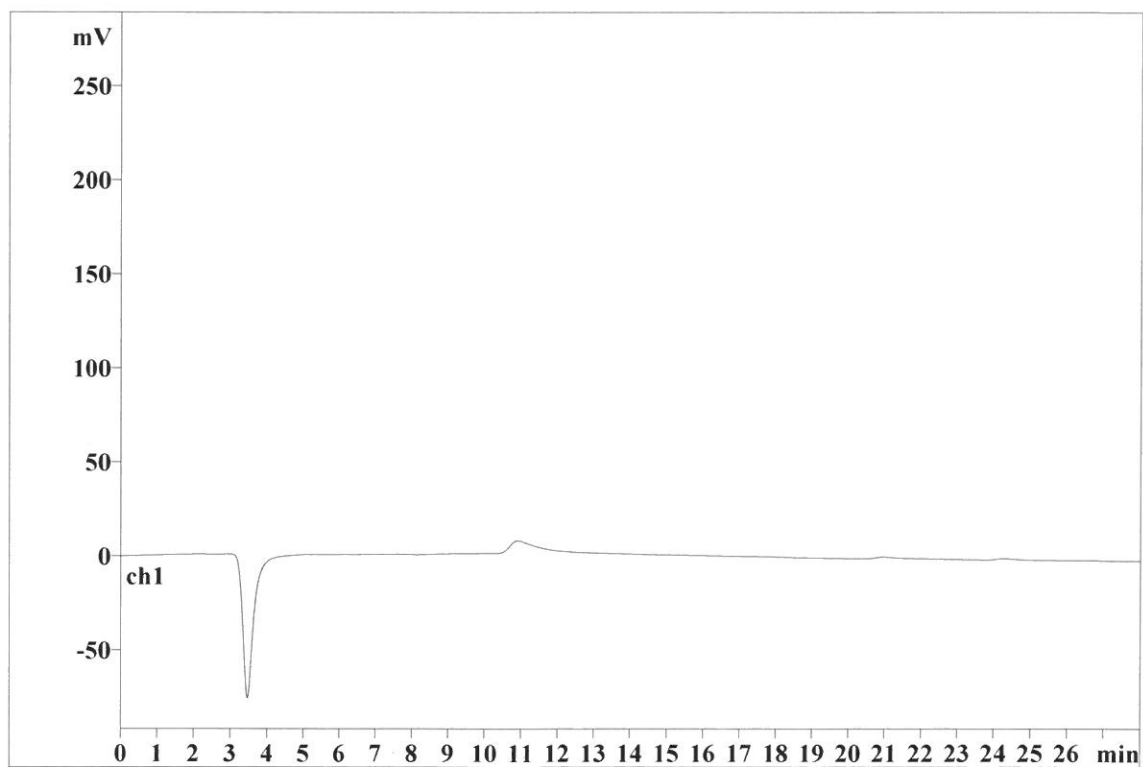

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:20:58 AM
Printed by: wet


Ident: LB105569BLW
Analysis from: 10/8/2019 11:27:58 AM
File: _2019-10-08_

Last save: 10/9/2019 9:20:21 AM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22711

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

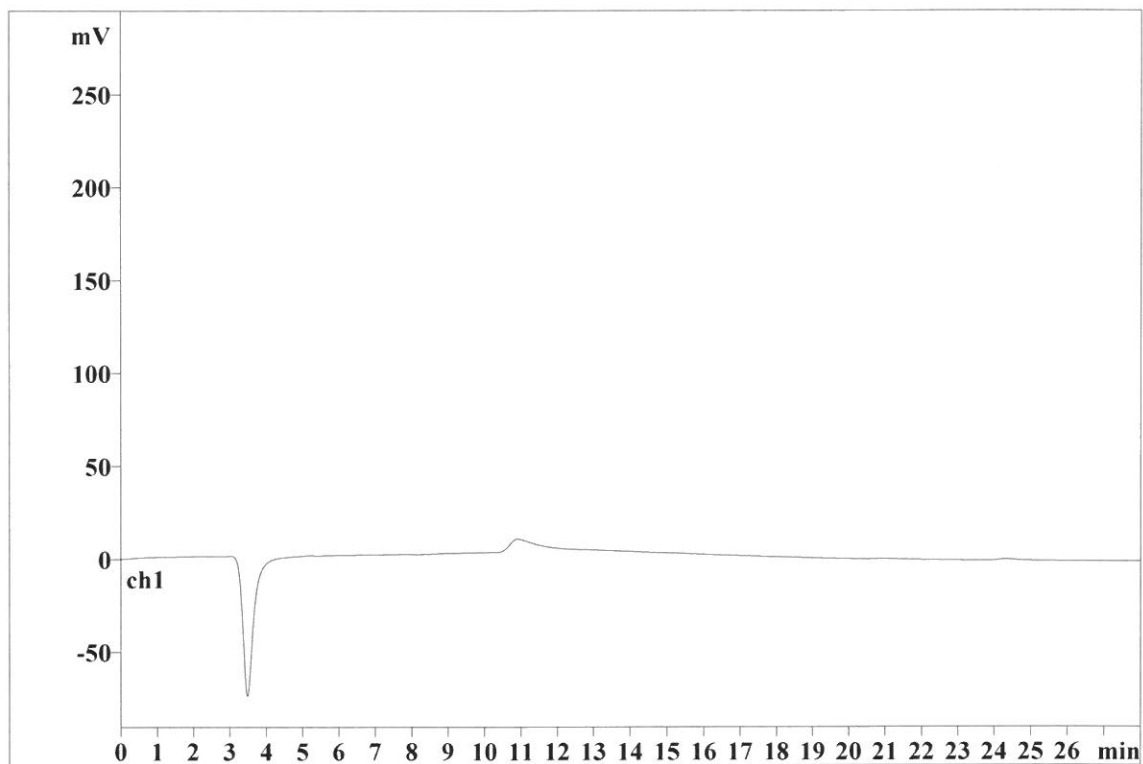

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:21:09 AM
Printed by: wet


Ident: LB105569BSW
Analysis from: 10/8/2019 11:58:57 AM
File: _2019-10-08_

Last save: 10/9/2019 9:20:21 AM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22712

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

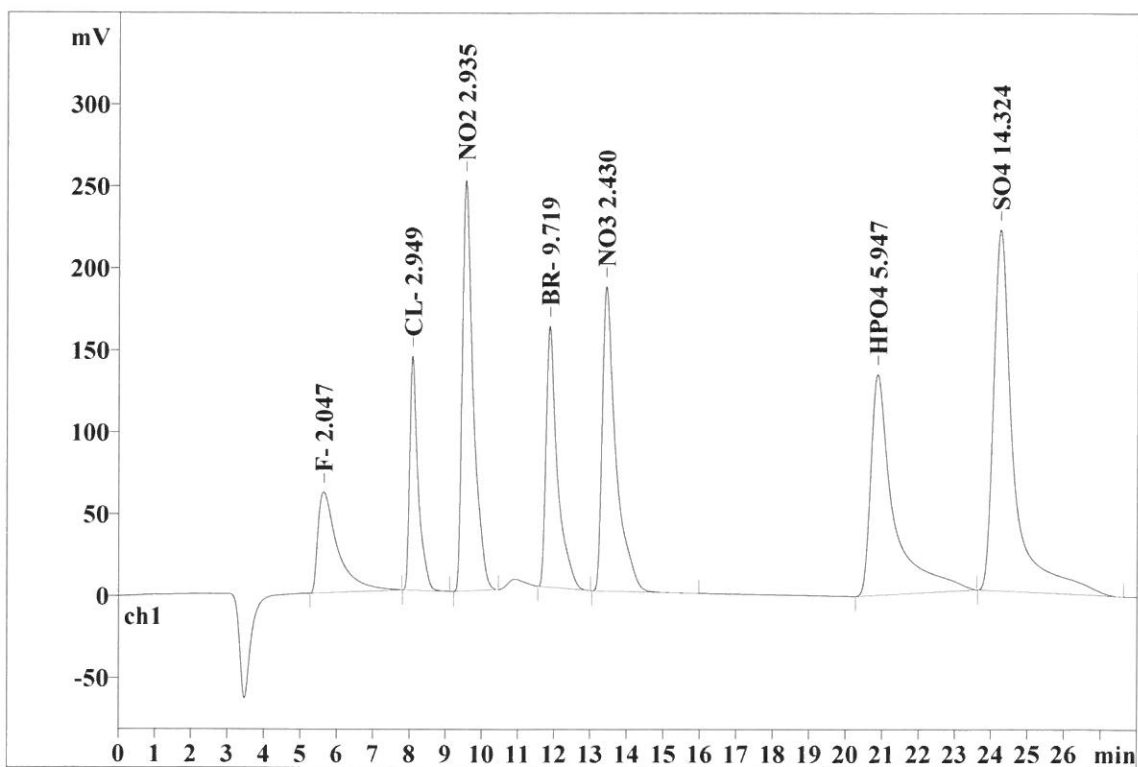

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.515	61.51	5.32	2334.015	7.13
2	8.06	0.229	142.94	12.37	2335.719	7.14
3	9.53	0.305	250.58	21.68	5286.094	16.15
4	11.86	0.291	159.47	13.80	3439.621	10.51
5	13.42	0.357	185.91	16.09	4856.172	14.84
6	20.86	0.513	134.80	11.66	5888.574	18.00
7	24.25	0.486	220.48	19.08	8581.111	26.22
7	28.00	0.385	1155.69	100.00	32721.306	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:21:24 AM
Printed by: wet


Ident: K5260-02
Analysis from: 10/8/2019 2:19:00 PM
File: _2019-10-08_

Last save: 10/8/2019 2:47:00 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22714

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

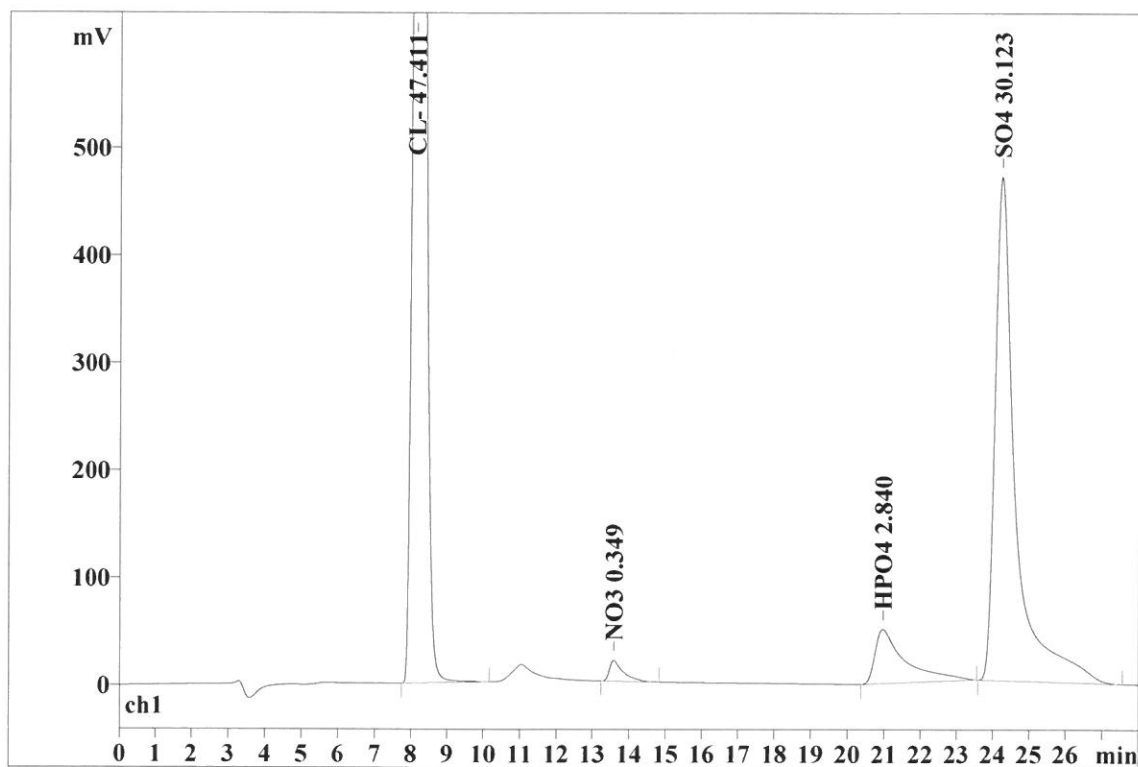

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.10	0.300	1915.53	78.04	38869.031	64.07
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.58	0.369	19.43	0.79	513.419	0.85
6	20.96	0.705	50.36	2.05	2913.972	4.80
7	24.23	0.489	468.76	19.10	18371.824	30.28
7	28.00	0.266	2454.08	99.99	60668.246	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:21:45 AM
Printed by: wet


Ident: K5260-03
Analysis from: 10/8/2019 2:49:58 PM
File: _2019-10-08_

Last save: 10/8/2019 3:17:59 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22715

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

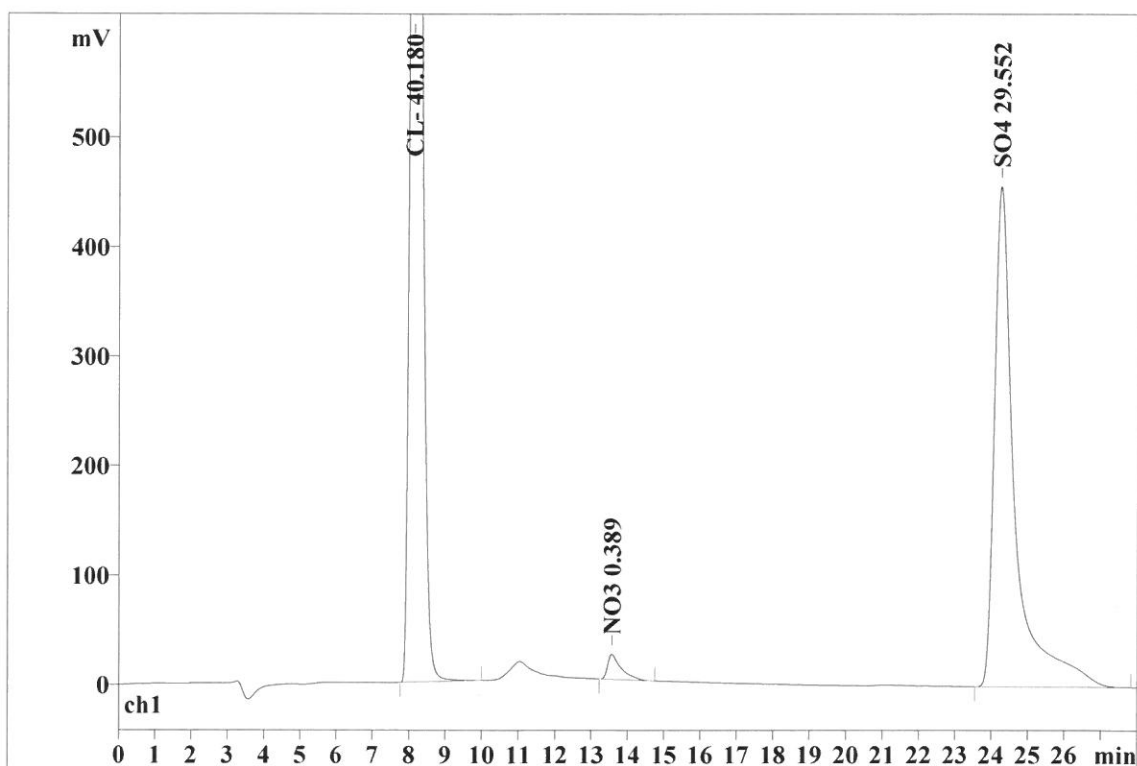

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.11	0.259	1877.86	79.66	32927.331	63.88
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.56	0.367	22.87	0.97	597.453	1.16
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.26	0.490	456.73	19.37	18017.912	34.96
7	28.00	0.159	2357.46	100.00	51542.695	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:21:59 AM
Printed by: wet


Ident: K5260-06
Analysis from: 10/8/2019 3:20:59 PM
File: _2019-10-08_

Last save: 10/8/2019 3:49:00 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22716

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

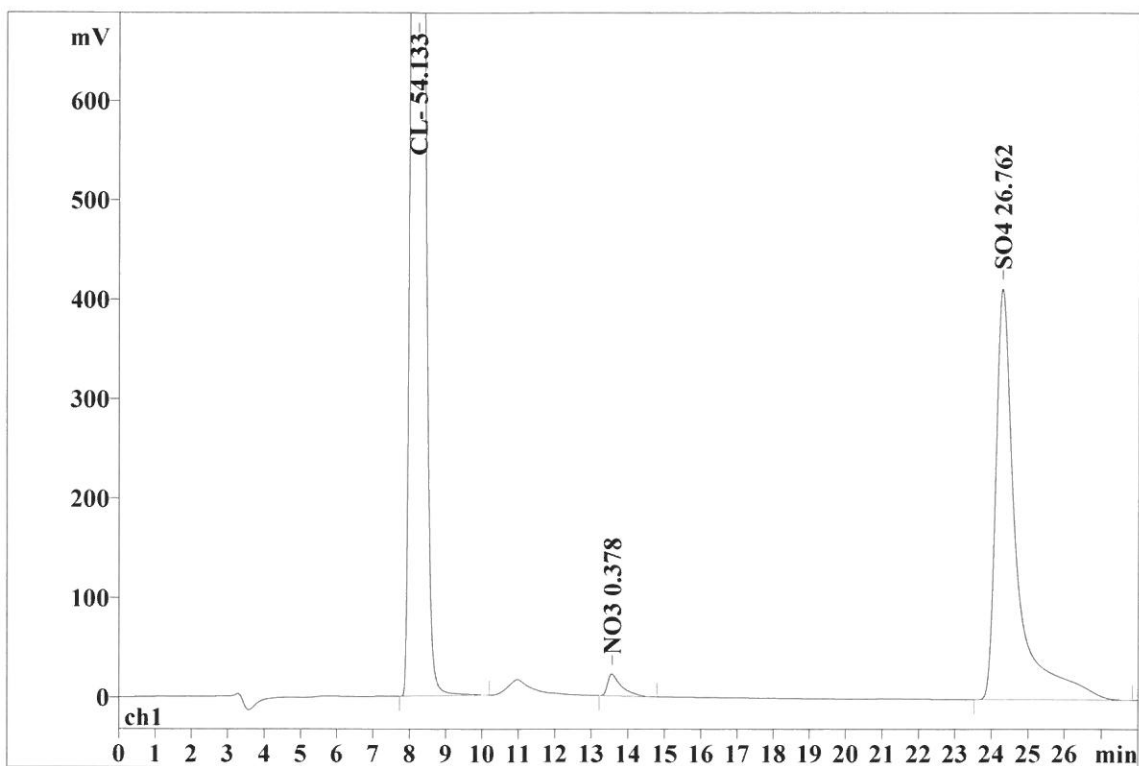

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.20	0.348	1916.99	81.48	44391.896	72.47
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.56	0.363	22.06	0.94	573.589	0.94
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.29	0.490	413.35	17.57	16289.205	26.59
7	28.00	0.171	2352.40	99.99	61254.689	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:22:30 AM
Printed by: wet


Ident: K5260-07
Analysis from: 10/8/2019 3:51:58 PM
File: _2019-10-08_

Last save: 10/8/2019 4:19:58 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22717

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

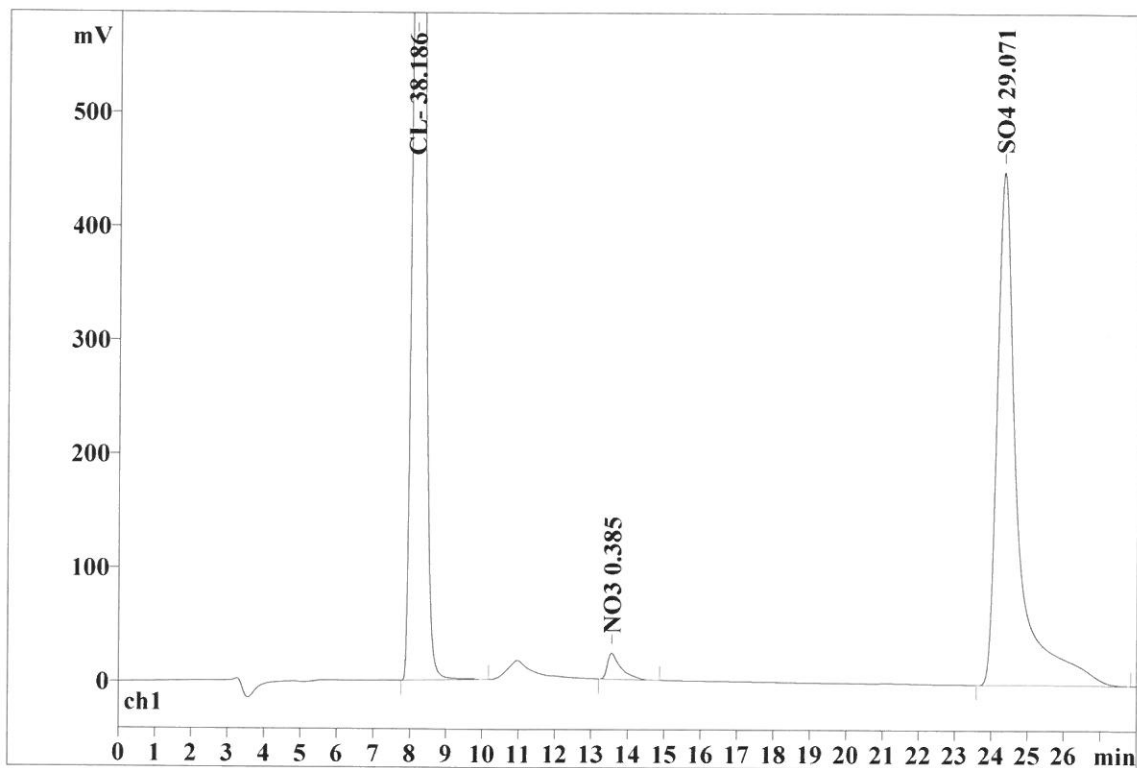

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.11	0.255	1804.54	79.24	31289.141	63.09
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.56	0.360	22.79	1.00	588.075	1.19
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.31	0.491	450.04	19.76	17719.785	35.73
7	28.00	0.158	2277.37	100.00	49597.001	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:22:46 AM
Printed by: wet


Ident: K5260-08
Analysis from: 10/8/2019 4:22:56 PM
File: _2019-10-08_

Last save: 10/8/2019 4:50:56 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22718

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

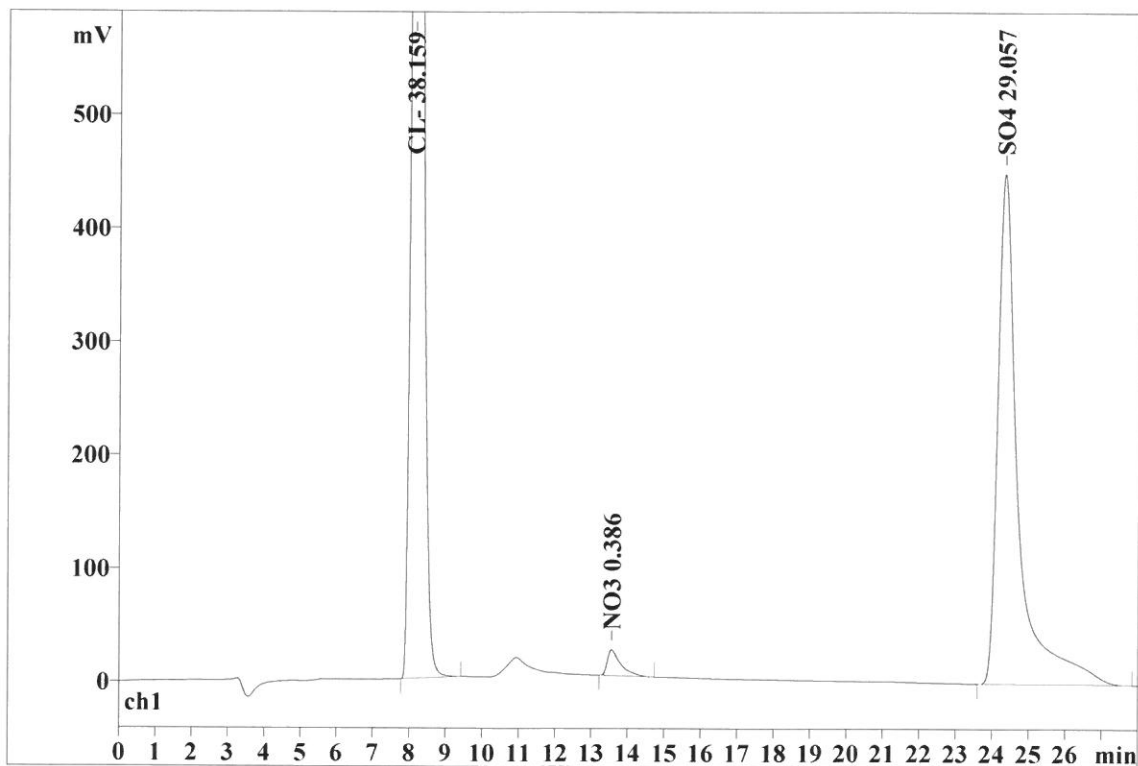

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.11	0.254	1811.64	79.30	31266.787	63.08
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.56	0.360	22.91	1.00	591.391	1.19
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.31	0.492	449.87	19.69	17711.585	35.73
7	28.00	0.158	2284.42	100.00	49569.763	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:22:59 AM
Printed by: wet


Ident: K5260-09
Analysis from: 10/8/2019 4:53:55 PM
File: _2019-10-08_

Last save: 10/8/2019 5:21:55 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22719

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

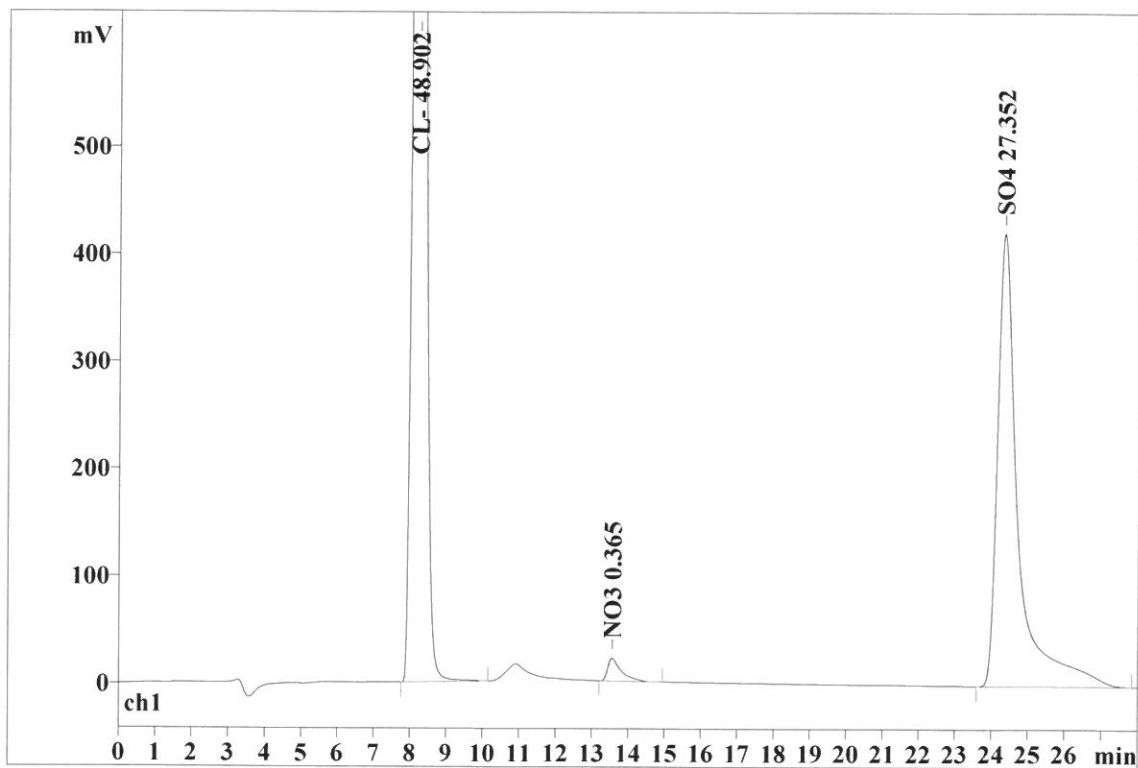

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.19	0.307	1922.52	81.45	40094.005	69.98
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.56	0.358	21.20	0.90	547.402	0.96
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.34	0.493	421.79	17.87	16654.825	29.07
7	28.00	0.165	2365.51	100.22	57296.233	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 12:57:46 PM
Printed by: wet


Ident: K5260-10
Analysis from: 10/8/2019 5:24:54 PM
File: _2019-10-08_

Last save: 10/9/2019 8:38:47 AM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22720

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

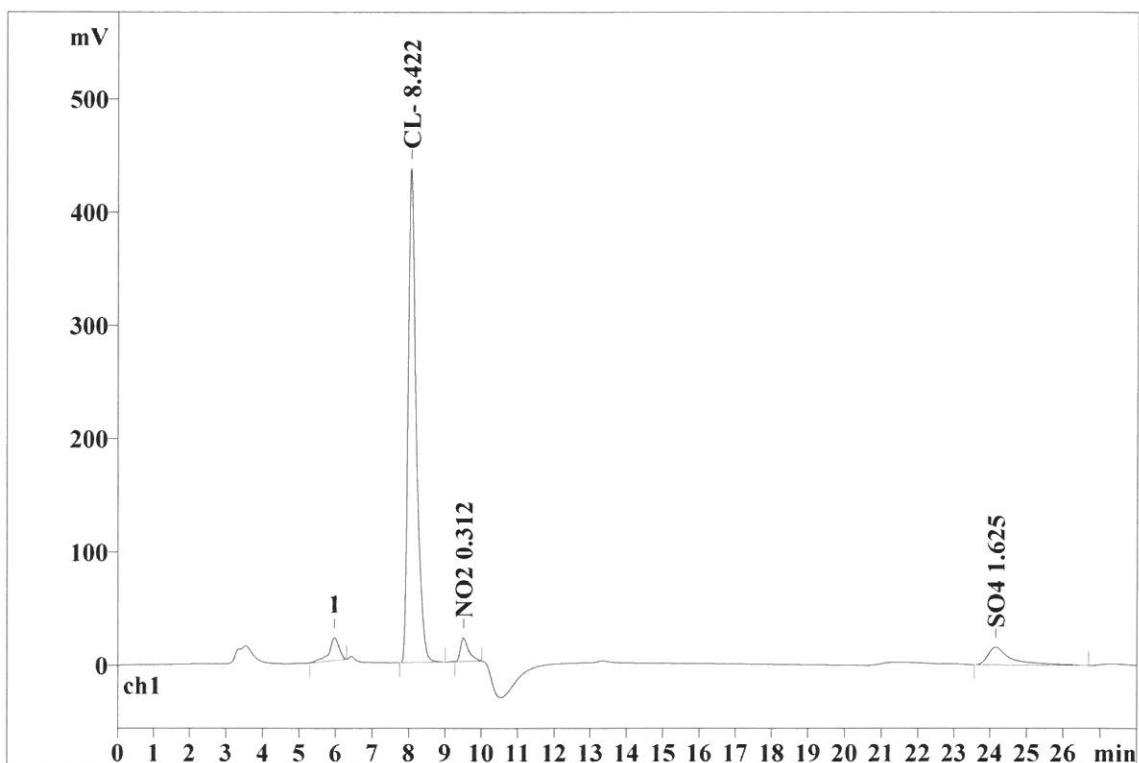

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.05	0.228	436.54	88.49	6832.837	82.62
3	9.51	0.232	20.95	4.25	336.404	4.07
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.16	0.552	15.62	3.17	711.714	8.61
7	28.00	0.144	473.10	95.90	7880.954	95.30

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:24:09 AM
Printed by: wet


Ident: K5260-11
Analysis from: 10/8/2019 5:55:54 PM
File: _2019-10-08_

Last save: 10/9/2019 9:24:04 AM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22721

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

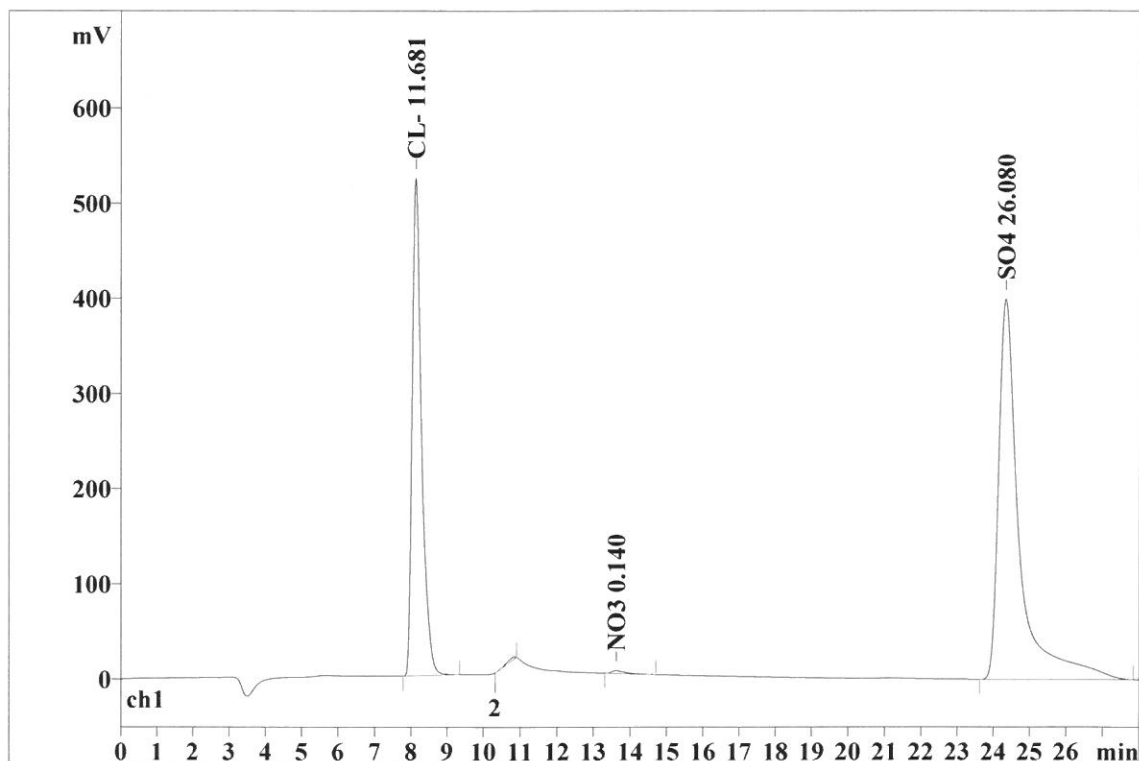

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.11	0.266	522.90	56.49	9510.971	37.31
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.62	0.357	3.07	0.33	77.765	0.31
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.34	0.497	399.68	43.18	15866.232	62.24
7	28.00	0.160	925.65	100.00	25454.969	99.86

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:24:45 AM
Printed by: wet


Ident: CCV
Analysis from: 10/8/2019 6:26:59 PM
File: _2019-10-08_

Last save: 10/8/2019 6:54:59 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22722

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

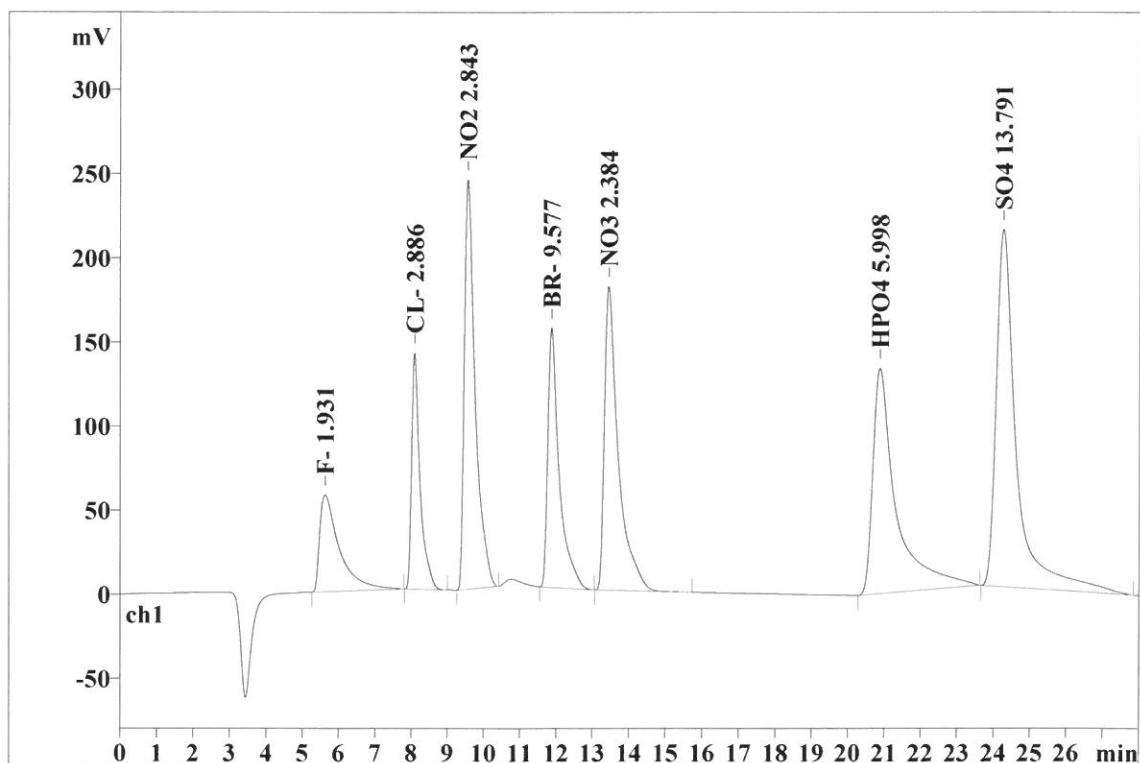

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.519	57.59	5.13	2196.199	6.88
2	8.07	0.225	140.42	12.51	2283.722	7.15
3	9.54	0.301	243.42	21.68	5113.678	16.02
4	11.86	0.293	154.34	13.75	3387.358	10.61
5	13.44	0.357	180.54	16.08	4760.148	14.91
6	20.89	0.534	133.90	11.93	5937.190	18.59
7	24.28	0.500	212.36	18.92	8251.354	25.84
7	28.00	0.390	1122.57	99.99	31929.649	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:25:01 AM
Printed by: wet


Ident: CCB
Analysis from: 10/8/2019 6:57:56 PM
File: _2019-10-08_

Last save: 10/8/2019 7:25:56 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22723

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

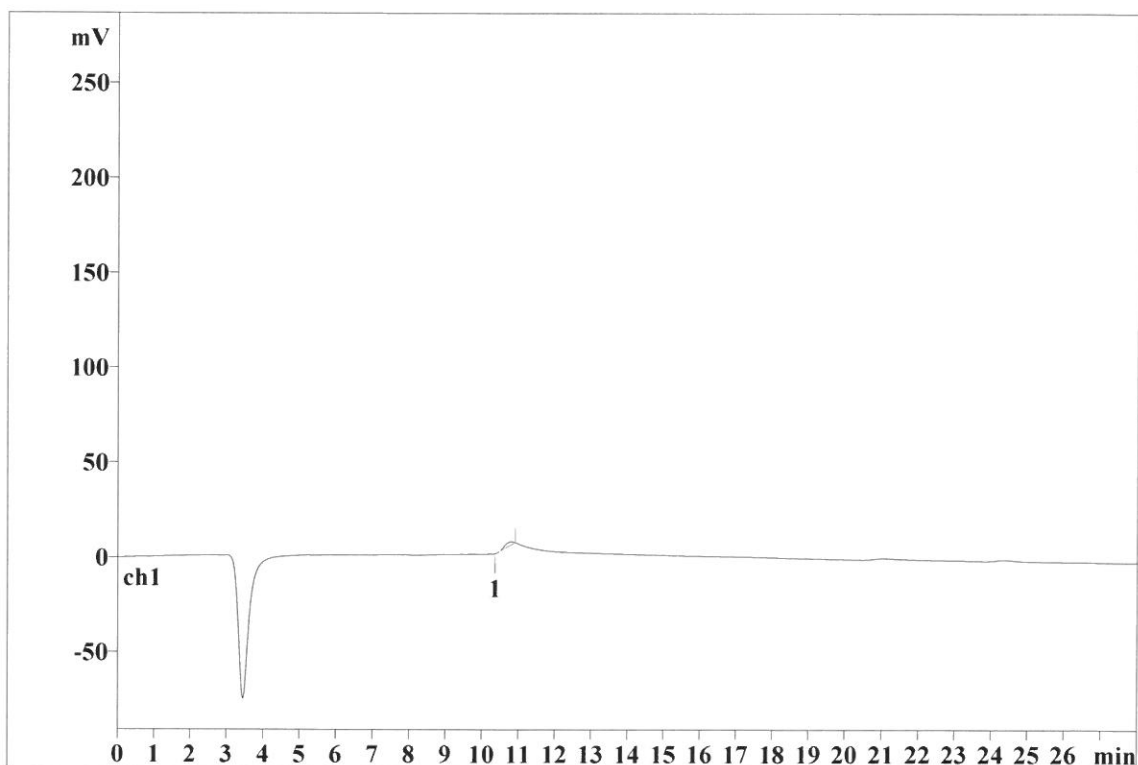

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.000	0.00	0.00	0.000	0.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:25:16 AM
Printed by: wet


Ident: K5260-12
Analysis from: 10/8/2019 7:29:01 PM
File: _2019-10-08_

Last save: 10/8/2019 7:57:02 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22724

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

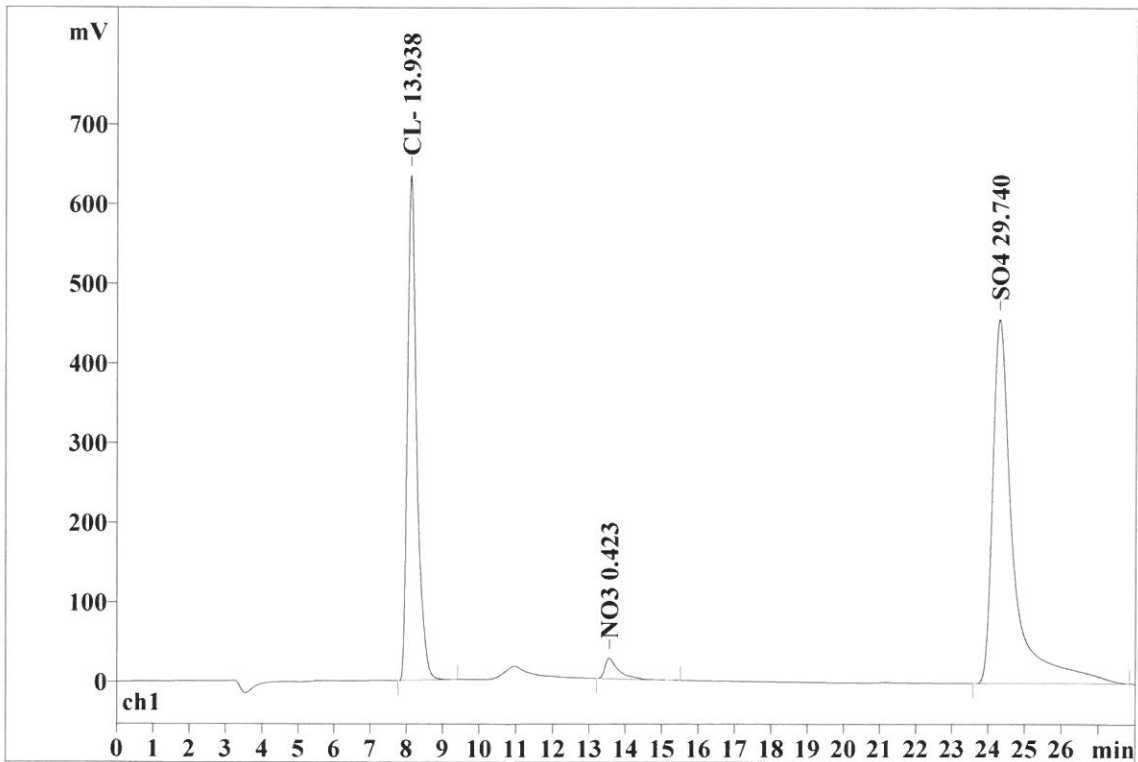

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.10	0.259	634.77	56.80	11364.917	37.67
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.54	0.358	25.47	2.28	667.166	2.21
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.31	0.498	457.22	40.91	18134.906	60.12
7	28.00	0.159	1117.47	100.00	30166.989	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:25:28 AM
Printed by: wet


Ident: K5260-13
Analysis from: 10/8/2019 8:00:00 PM
File: _2019-10-08_

Last save: 10/8/2019 8:28:00 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22725

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

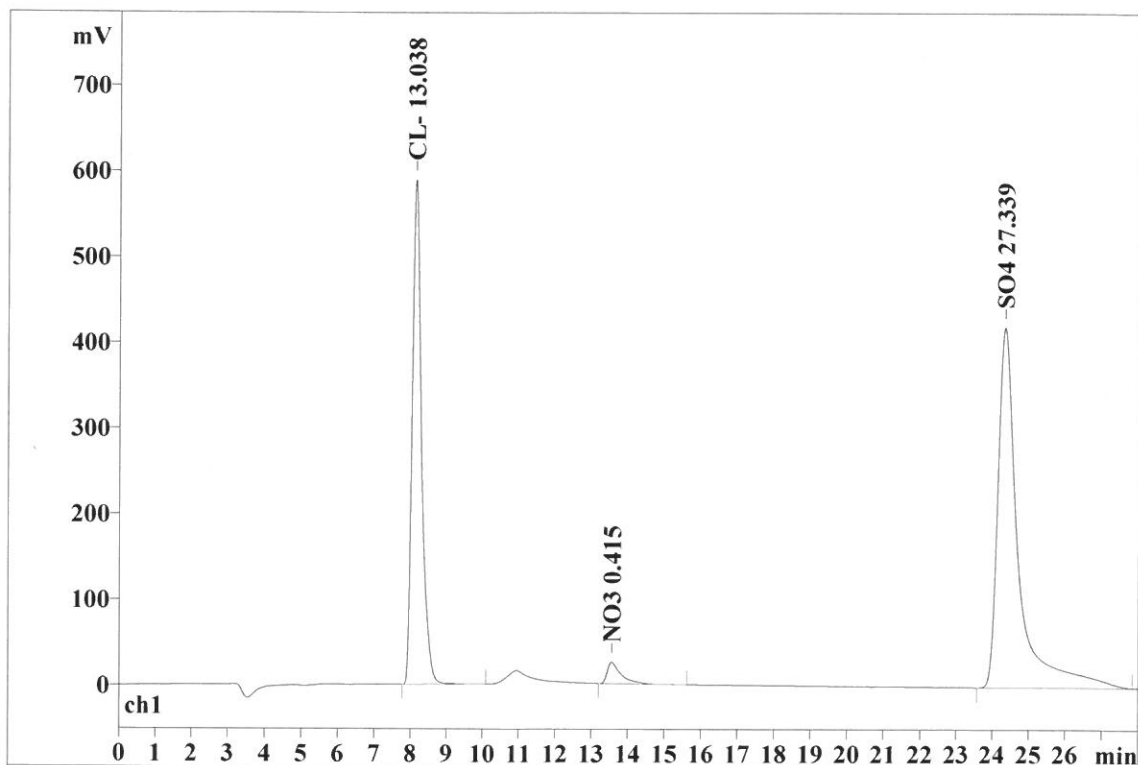

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.11	0.263	588.86	56.97	10625.948	38.05
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.56	0.357	24.90	2.41	651.427	2.33
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.33	0.498	419.84	40.62	16646.779	59.61
7	28.00	0.160	1033.61	99.99	27924.154	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:25:45 AM
Printed by: wet


Ident: K5260-03DUP
Analysis from: 10/8/2019 8:31:05 PM
File: _2019-10-08_

Last save: 10/8/2019 8:59:06 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22726

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

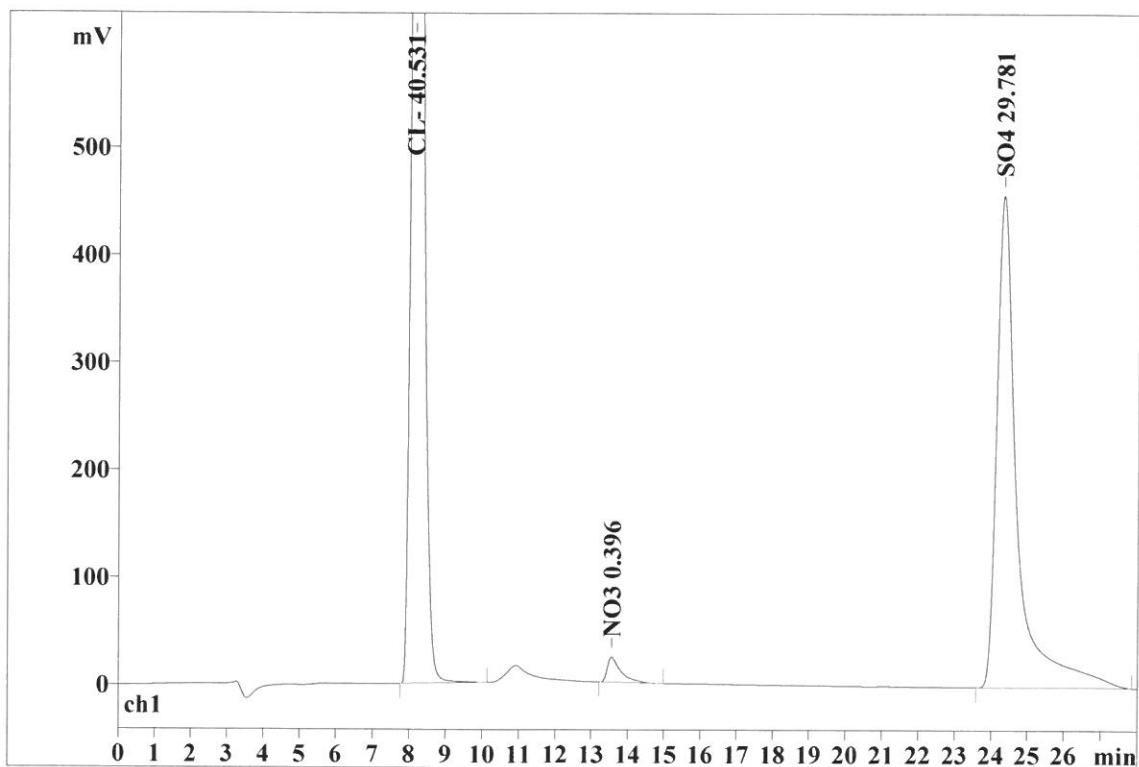

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.12	0.249	1918.81	80.05	33215.375	63.89
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	13.56	0.358	23.41	0.98	610.881	1.18
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.33	0.499	458.01	19.11	18159.907	34.93
7	28.00	0.158	2400.23	100.13	51986.163	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:25:56 AM
Printed by: wet


Ident: K5260-04MS
Analysis from: 10/8/2019 9:02:05 PM
File: _2019-10-08_

Last save: 10/8/2019 9:30:06 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22727

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

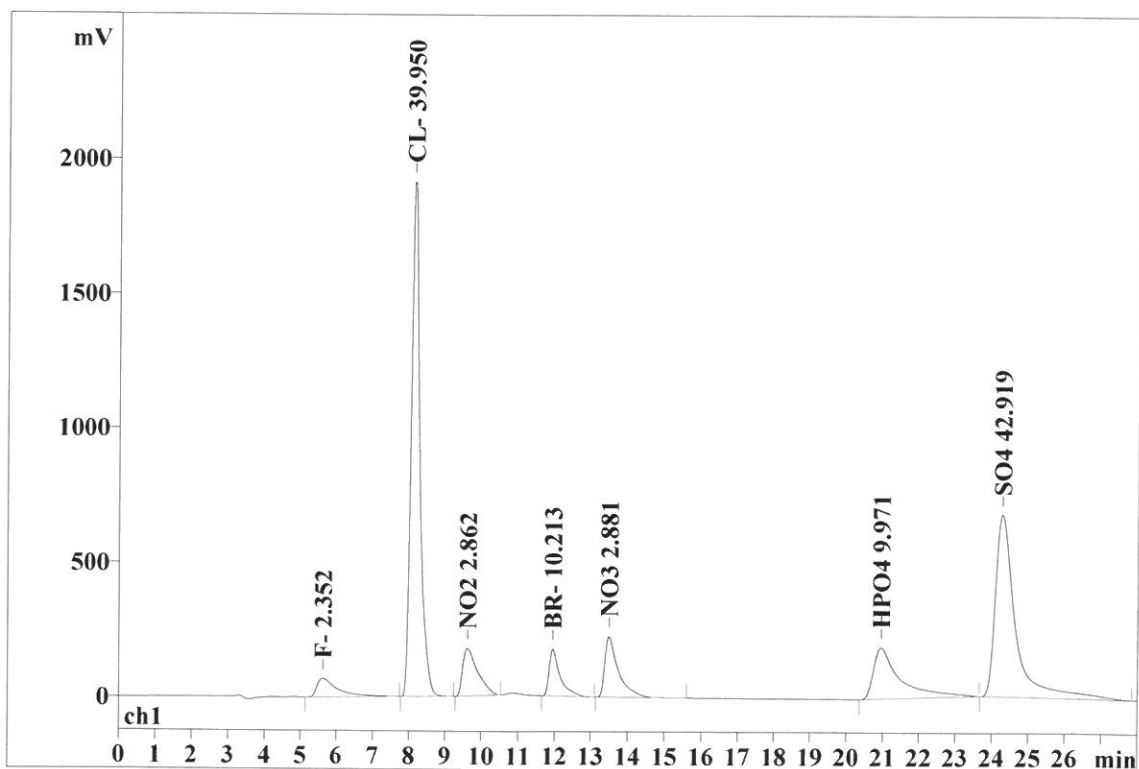

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.533	68.16	1.99	2695.137	3.13
2	8.11	0.244	1914.46	55.91	32738.626	38.05
3	9.61	0.444	176.64	5.16	5149.851	5.99
4	11.95	0.277	174.25	5.09	3621.837	4.21
5	13.49	0.351	225.29	6.58	5797.971	6.74
6	20.95	0.613	189.87	5.54	9740.163	11.32
7	24.29	0.501	676.42	19.75	26301.768	30.57
7	28.00	0.423	3425.09	100.03	86045.353	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:26:11 AM
Printed by: wet


Ident: K5260-05MSD
Analysis from: 10/8/2019 9:33:05 PM
File: _2019-10-08_

Last save: 10/8/2019 10:01:05 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22728

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

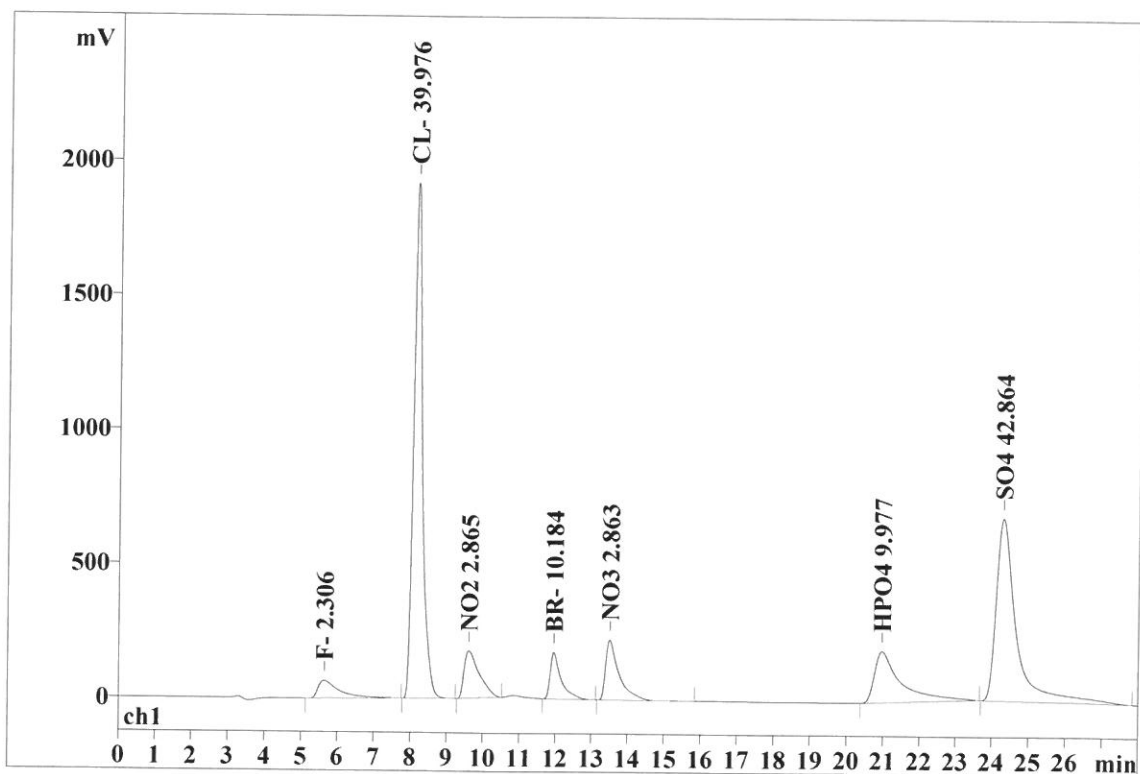

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.64	0.550	65.49	1.91	2640.641	3.07
2	8.12	0.244	1917.76	56.05	32759.682	38.12
3	9.61	0.447	176.07	5.15	5154.197	6.00
4	11.96	0.278	172.91	5.05	3611.427	4.20
5	13.50	0.351	223.07	6.52	5759.563	6.70
6	20.96	0.613	190.22	5.56	9745.680	11.34
7	24.30	0.500	677.84	19.81	26267.795	30.57
7	28.00	0.426	3423.37	100.05	85938.985	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:26:27 AM
Printed by: wet


Ident: CCV
Analysis from: 10/8/2019 10:04:09 PM
File: _2019-10-08_

Last save: 10/8/2019 10:32:09 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22729

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

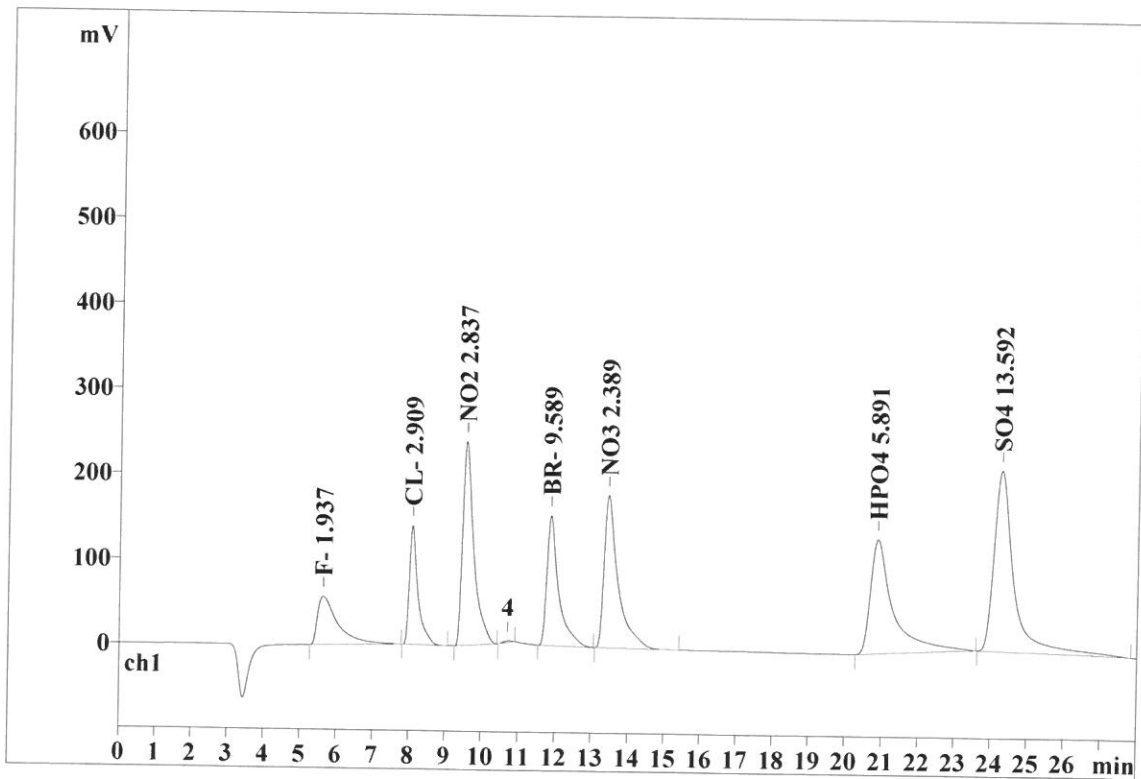

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.528	56.74	5.09	2202.921	6.94
2	8.07	0.226	139.77	12.53	2303.215	7.25
3	9.54	0.306	239.16	21.44	5101.763	16.06
4	11.86	0.296	152.46	13.67	3392.002	10.68
5	13.43	0.358	178.90	16.04	4771.306	15.02
6	20.87	0.532	133.89	12.01	5834.621	18.37
7	24.27	0.499	212.31	19.04	8127.473	25.59
7	28.00	0.392	1113.23	99.81	31733.301	99.90

This report has been created by IC Net
METROHM LTD

Report date: 10/9/2019 9:26:40 AM
Printed by: wet


Ident: CCB
Analysis from: 10/8/2019 10:35:08 PM
File: _2019-10-08_

Last save: 10/8/2019 11:03:08 PM

Method: AnionsIC2-100119.mtw
Run operator: wet
Analysis number: 22730

Last save: 10/1/2019 3:21:

SAMPLE:
: CT/AP
Vial number: 22
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

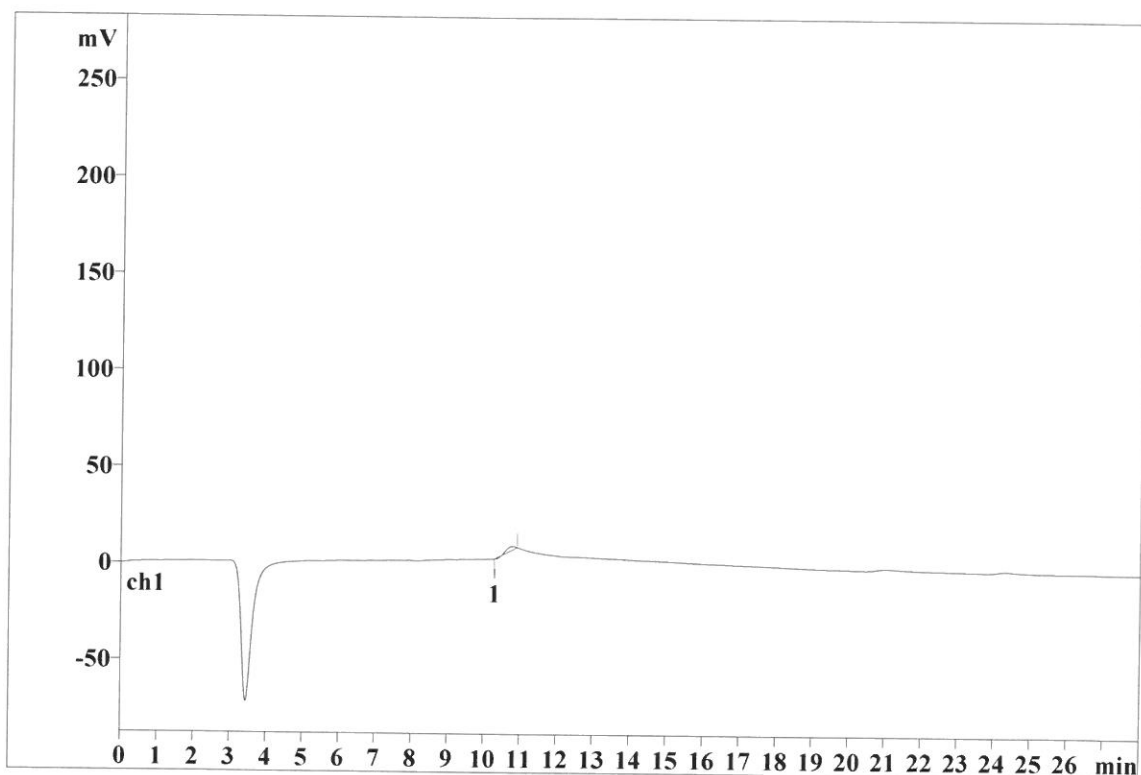

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.000	0.00	0.00	0.000	0.00

This report has been created by IC Net
METROHM LTD