

LB105759

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : 07

Instrument ID : Konelab

10/17/2019 9:49

Test

Reactive
~~Total~~ CN

Accepted

10/17/2019 8:27

Factor

1162


Bias

0.001

Coeff. of det.

0.999975

Errors

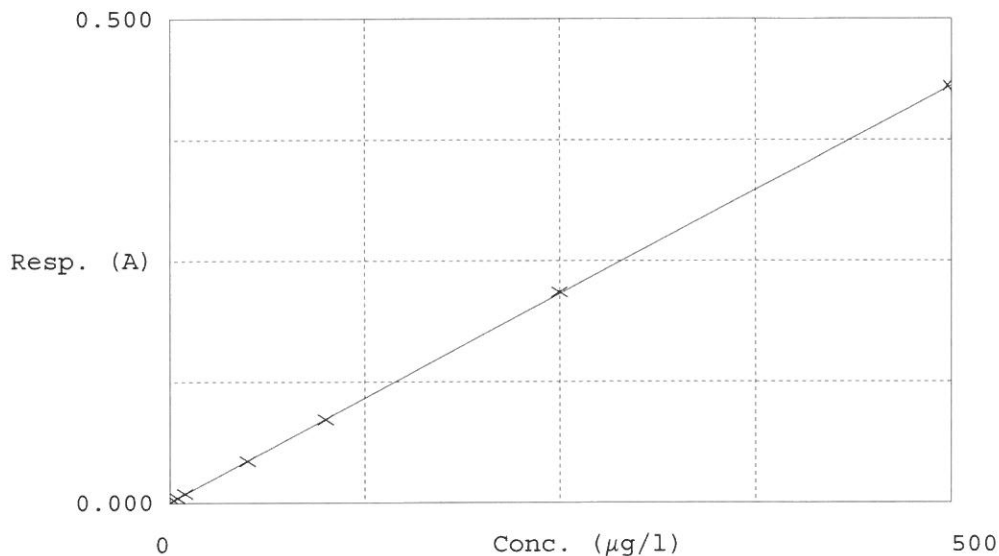

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.2710	0.0000	
2	5.0PPBCN	0.005	5.0379	5.0000	
3	10PPBCN	0.010	10.1507	10.0000	
4	50PPBCN	0.043	49.2638	50.0000	
5	100PPBCN	0.086	99.1312	100.0000	
6	250PPBCN	0.218	251.8026	250.0000	
7	500PPBCN	0.431	499.3427	500.0000	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

10/17/2019 9:49

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.802	0.0	0.085	
ICB1	0.682	0.0	0.002	
CCV1	252.808	0.0	0.219	
CCB1	0.646	0.0	0.001	
PB124039BL	1.110	0.0	0.002	
K5152-09	0.397	0.0	0.001	
K5152-09DUP	0.442	0.0	0.001	
K5392-04	0.345	0.0	0.001	
K5392-08	0.403	0.0	0.001	
CCV2	256.625	0.0	0.222	
CCB2	0.585	0.0	0.001	

N	11
Mean	55.622
SD	102.6180
CV%	184.49

CT
10/17/19

Aquakem v. 7.2AQ1

Results from time period:

Thu Oct 17 09:44:07 2019

Thu Oct 17 09:44:17 2019

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.271	µg/l	10/17/2019 8:23:23	
5.0PPBCN	A	Reactive CN	P	5.0379	µg/l	10/17/2019 8:23:24	
10PPBCN	A	Reactive CN	P	10.1507	µg/l	10/17/2019 8:23:25	
50PPBCN	A	Reactive CN	P	49.2638	µg/l	10/17/2019 8:23:26	
100PPBCN	A	Reactive CN	P	99.1312	µg/l	10/17/2019 8:23:27	
250PPBCN	A	Reactive CN	P	251.8026	µg/l	10/17/2019 8:23:28	
500PPBCN	A	Reactive CN	P	499.3427	µg/l	10/17/2019 8:23:29	
ICV1	S	Reactive CN	P	97.8021	µg/l	10/17/2019 9:44:07	
ICB1	S	Reactive CN	P	0.6819	µg/l	10/17/2019 9:44:08	
CCV1	S	Reactive CN	P	252.8079	µg/l	10/17/2019 9:44:09	
CCB1	S	Reactive CN	P	0.6455	µg/l	10/17/2019 9:44:10	
PB124039BL	S	Reactive CN	P	1.1096	µg/l	10/17/2019 9:44:11	
K5152-09	S	Reactive CN	P	0.3968	µg/l	10/17/2019 9:44:12	
K5152-09DUP	S	Reactive CN	P	0.4418	µg/l	10/17/2019 9:44:13	
K5392-04	S	Reactive CN	P	0.3446	µg/l	10/17/2019 9:44:14	
K5392-08	S	Reactive CN	P	0.4034	µg/l	10/17/2019 9:44:15	
CCV2	S	Reactive CN	P	256.6252	µg/l	10/17/2019 9:44:16	
CCB2	S	Reactive CN	P	0.5847	µg/l	10/17/2019 9:44:17	