

LB105790

=====

Calibration results	Aquakem 7.2AQ1	Page: 1
---------------------	----------------	---------

=====

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CF

Instrument ID : Konelab

10/18/2019 12:22


Test Reactive
~~Total~~ CN

Accepted 10/18/2019 12:22

Factor 1121
Bias 0.001

Coeff. of det. 0.999919

Errors

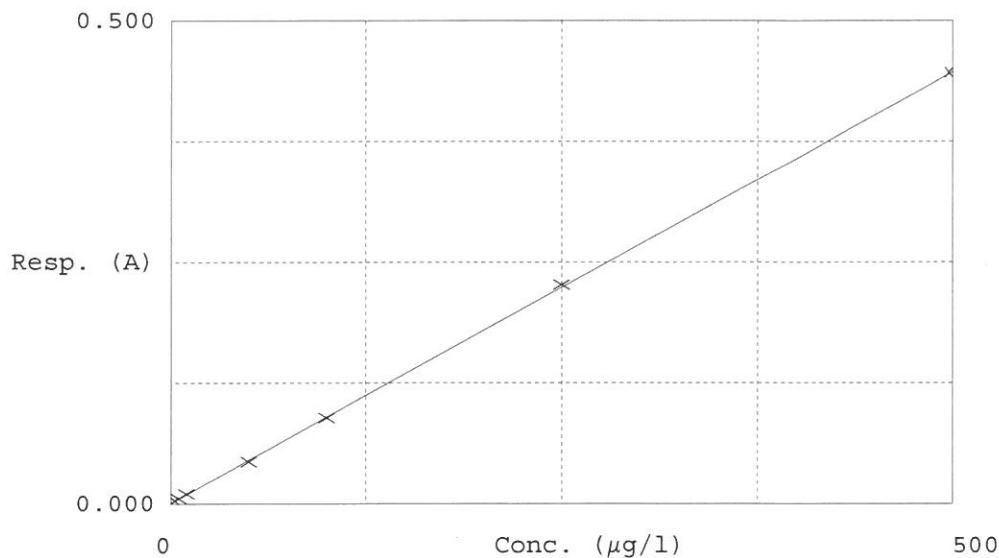

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.8163	0.0000	
2	5.0PPBCN	0.006	5.1734	5.0000	
3	10PPBCN	0.010	10.6206	10.0000	
4	50PPBCN	0.044	47.8300	50.0000	
5	100PPBCN	0.089	98.6564	100.0000	
6	250PPBCN	0.227	252.8636	250.0000	
7	500PPBCN	0.446	499.0398	500.0000	

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : G

Instrument ID : Konelab

10/18/2019 12:47

Test: ^{Reactive}
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	92.394 ✓	0.0	0.083	
ICB1	0.649 ✓	0.0	0.002	
CCV1	239.199 ✓	0.0	0.214	
CCB1	0.612 ✓	0.0	0.002	
PB124111BL	0.295	0.0	0.001	
K5153-04	0.352	0.0	0.001	
K5153-04DUP	0.319	0.0	0.001	
K5439-02	0.287	0.0	0.001	
K5439-03	0.528	0.0	0.001	
CCV2	240.592 ✓	0.0	0.216	
CCB2	0.483 ✓	0.0	0.001	
N	11			
Mean	52.337			
SD	96.6996			
CV%	184.76			

CT
10/18/19

Aquakem v. 7.2AQ1

Results from time period:

Fri Oct 18 12:02:28 2019

Fri Oct 18 12:46:17 2019

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Reactive CN	P	0.8163	µg/l	10/18/2019 12:21:36
5.OPPBCN	A	Reactive CN	P	5.1734	µg/l	10/18/2019 12:21:37
10PPBCN	A	Reactive CN	P	10.6206	µg/l	10/18/2019 12:21:38
50PPBCN	A	Reactive CN	P	47.83	µg/l	10/18/2019 12:21:39
100PPBCN	A	Reactive CN	P	98.6564	µg/l	10/18/2019 12:21:40
250PPBCN	A	Reactive CN	P	252.8636	µg/l	10/18/2019 12:21:41
500PPBCN	A	Reactive CN	P	499.0398	µg/l	10/18/2019 12:21:42
ICV1	S	Reactive CN	P	92.3942	µg/l	10/18/2019 12:46:07
ICB1	S	Reactive CN	P	0.6491	µg/l	10/18/2019 12:46:08
CCV1	S	Reactive CN	P	239.1992	µg/l	10/18/2019 12:46:09
CCB1	S	Reactive CN	P	0.6116	µg/l	10/18/2019 12:46:10
PB124111BL	S	Reactive CN	P	0.2954	µg/l	10/18/2019 12:46:11
K5153-04	S	Reactive CN	P	0.3522	µg/l	10/18/2019 12:46:12
K5153-04DUP	S	Reactive CN	P	0.3186	µg/l	10/18/2019 12:46:13
K5439-02	S	Reactive CN	P	0.2868	µg/l	10/18/2019 12:46:14
K5439-03	S	Reactive CN	P	0.5283	µg/l	10/18/2019 12:46:15
CCV2	S	Reactive CN	P	240.5921	µg/l	10/18/2019 12:46:16
CCB2	S	Reactive CN	P	0.4831	µg/l	10/18/2019 12:46:17