

LB106105

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AL

Instrument ID : Konelab

11/5/2019 11:50

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.410	0.0	0.086	
ICB1	-0.491	0.0	0.002	
CCV1	237.831	0.0	0.212	
CCB1	-0.590	0.0	0.002	
PB124520BL	-0.686	0.0	0.002	
K5658-04	-1.412	0.0	0.001	
K5658-04DUP	-0.489	0.0	0.002	
K5658-08	-0.818	0.0	0.001	
K5676-05	-0.697	0.0	0.002	
PB124522BL	-0.486	0.0	0.002	
K5623-03	-0.779	0.0	0.001	
K5623-03DUP	-0.672	0.0	0.002	
CCV2	257.865	0.0	0.230	
CCB2	-0.552	0.0	0.002	

N	14
Mean	41.603
SD	91.0395
CV%	218.83

AD

Aquakem v. 7.2AQ1

Results from time period:

Tue Nov 05 08:47:04 2019

Tue Nov 05 11:47:58 2019

Sample Id	Sam/Ctr/c/	Test short Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive Cl P	-0.9263	µg/l	11/5/2019 11:14:27	
5.OPPBCN	A	Reactive Cl P	4.8367	µg/l	11/5/2019 11:14:28	
10PPBCN	A	Reactive Cl P	9.6966	µg/l	11/5/2019 11:14:29	
50PPBCN	A	Reactive Cl P	50.0101	µg/l	11/5/2019 11:14:30	
100PPBCN	A	Reactive Cl P	100.0271	µg/l	11/5/2019 11:14:31	
250PPBCN	A	Reactive Cl P	252.7091	µg/l	11/5/2019 11:14:32	
500PPBCN	A	Reactive Cl P	498.6468	µg/l	11/5/2019 11:14:33	
ICV1	S	Reactive Cl P	94.4103	µg/l	11/5/2019 11:44:05	
ICB1	S	Reactive Cl P	-0.4908	µg/l	11/5/2019 11:44:06	
CCV1	S	Reactive Cl P	237.8307	µg/l	11/5/2019 11:44:07	
CCB1	S	Reactive Cl P	-0.5902	µg/l	11/5/2019 11:44:08	
PB124520BL	S	Reactive Cl P	-0.6858	µg/l	11/5/2019 11:44:09	
K5658-04	S	Reactive Cl P	-1.4116	µg/l	11/5/2019 11:44:10	
K5658-04DUP	S	Reactive Cl P	-0.4887	µg/l	11/5/2019 11:44:11	
K5658-08	S	Reactive Cl P	-0.8177	µg/l	11/5/2019 11:44:12	
K5676-05	S	Reactive Cl P	-0.6966	µg/l	11/5/2019 11:44:13	
PB124522BL	S	Reactive Cl P	-0.4858	µg/l	11/5/2019 11:44:14	
K5623-03	S	Reactive Cl P	-0.7787	µg/l	11/5/2019 11:44:15	
K5623-03DUP	S	Reactive Cl P	-0.6719	µg/l	11/5/2019 11:47:56	
CCV2	S	Reactive Cl P	257.8651	µg/l	11/5/2019 11:47:57	
CCB2	S	Reactive Cl P	-0.5522	µg/l	11/5/2019 11:47:58	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AC

Instrument ID : Konelab

11/5/2019 11:17


Test Total CN

Accepted 11/5/2019 11:17

Factor 1133
Bias 0.002

Coeff. of det. 0.999951

Errors

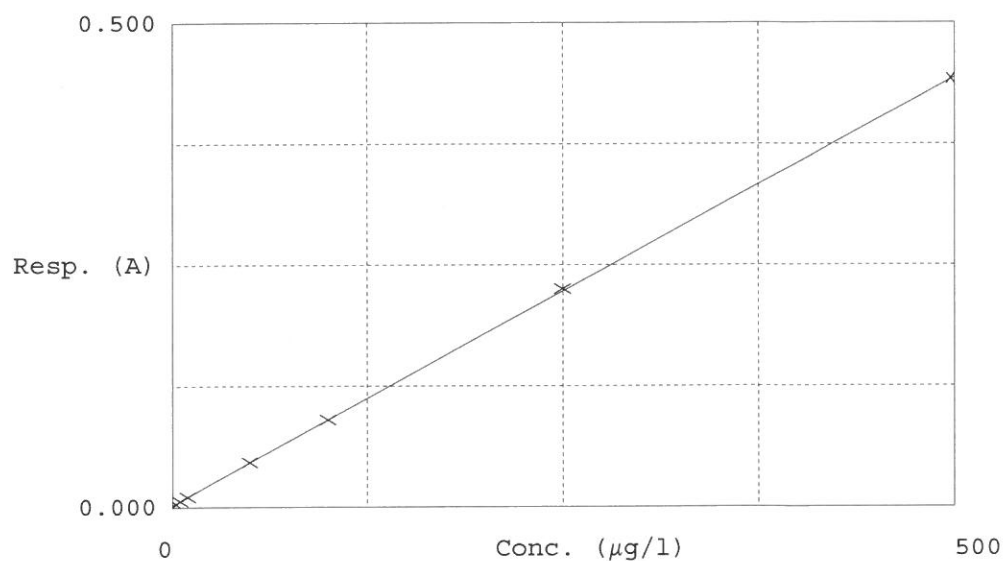

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.9263	0.0000	
2	5.0PPBCN	0.006	4.8367	5.0000	
3	10PPBCN	0.011	9.6966	10.0000	
4	50PPBCN	0.046	50.0101	50.0000	
5	100PPBCN	0.090	100.0271	100.0000	
6	250PPBCN	0.225	252.7091	250.0000	
7	500PPBCN	0.442	498.6468	500.0000	