

LB106200

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Ab

Instrument ID : Konelab

11/11/2019 15:00

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.698	0.0	0.087	
ICB1	0.807	0.0	0.003	
CCV1	244.294	0.0	0.218	
CCB1	0.749	0.0	0.003	
PB124695BL	0.766	0.0	0.003	
LOWPB124695	9.092	0.0	0.010	
HIGHPB124695	487.550	0.0	0.434	
K5673-01	-0.063	0.0	0.002	
K5673-01DUP	-0.643	0.0	0.002	
K5673-01MS	34.816	0.0	0.033	
K5673-01MSD	30.619	0.0	0.029	
K5676-11	-0.299	0.0	0.002	
K5730-01	0.455	0.0	0.003	
CCV2	243.621	0.0	0.218	
CCB2	0.673	0.0	0.003	
K5746-05	-0.620	0.0	0.002	
K5749-01	0.292	0.0	0.003	
K5760-02	-0.225	0.0	0.002	
K5760-12	-0.765	0.0	0.002	
K5760-07	-0.096	0.0	0.002	
PB124695BS	100.242	0.0	0.091	
CCV3	258.396	0.0	0.231	
CCB3	0.796	0.0	0.003	

N	23
Mean	65.485
SD	125.4659
CV%	191.60

AK

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 11 13:01:05 2019

Mon Nov 11 14:59:40 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.2441	µg/l	11/11/2019 13:01:05	
5.OPPBCN	A	Total CN	P	3.589	µg/l	11/11/2019 13:01:06	
10PPBCN	A	Total CN	P	9.8897	µg/l	11/11/2019 13:01:07	
50PPBCN	A	Total CN	P	49.2409	µg/l	11/11/2019 13:01:08	
100PPBCN	A	Total CN	P	100.2388	µg/l	11/11/2019 13:01:09	
250PPBCN	A	Total CN	P	254.4825	µg/l	11/11/2019 13:01:10	
500PPBCN	A	Total CN	P	497.8032	µg/l	11/11/2019 13:01:11	
ICV1	S	Total CN	P	95.6981	µg/l	11/11/2019 13:53:25	
ICB1	S	Total CN	P	0.8066	µg/l	11/11/2019 13:53:26	
CCV1	S	Total CN	P	244.2942	µg/l	11/11/2019 13:53:27	
CCB1	S	Total CN	P	0.7488	µg/l	11/11/2019 13:53:28	
PB124695BL	S	Total CN	P	0.7656	µg/l	11/11/2019 13:53:29	
LOWPB124695	S	Total CN	P	9.0918	µg/l	11/11/2019 13:53:31	
HIGHPB124695	S	Total CN	P	487.5497	µg/l	11/11/2019 13:53:32	
K5673-01	S	Total CN	P	-0.0635	µg/l	11/11/2019 13:53:33	
K5673-01DUP	S	Total CN	P	-0.6426	µg/l	11/11/2019 13:53:34	
K5673-01MS	S	Total CN	P	34.8161	µg/l	11/11/2019 13:53:35	
K5673-01MSD	S	Total CN	P	30.6192	µg/l	11/11/2019 14:00:57	
K5676-11	S	Total CN	P	-0.2992	µg/l	11/11/2019 14:00:58	
K5730-01	S	Total CN	P	0.455	µg/l	11/11/2019 14:00:59	
CCV2	S	Total CN	P	243.6205	µg/l	11/11/2019 14:01:00	
CCB2	S	Total CN	P	0.673	µg/l	11/11/2019 14:01:01	
K5746-05	S	Total CN	P	-0.62	µg/l	11/11/2019 14:01:02	
K5749-01	S	Total CN	P	0.2915	µg/l	11/11/2019 14:01:03	
K5760-02	S	Total CN	P	-0.2248	µg/l	11/11/2019 14:01:04	
K5760-12	S	Total CN	P	-0.7651	µg/l	11/11/2019 14:01:06	
K5760-07	S	Total CN	P	-0.0956	µg/l	11/11/2019 14:34:12	
PB124695BS	S	Total CN	P	100.2418	µg/l	11/11/2019 14:59:38	
CCV3	S	Total CN	P	258.3963	µg/l	11/11/2019 14:59:39	
CCB3	S	Total CN	P	0.7959	µg/l	11/11/2019 14:59:40	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AK

Instrument ID : Konelab

11/11/2019 13:21


Test Total CN

Accepted 11/11/2019 13:21

Factor 1130
Bias 0.002

Coeff. of det. 0.999866

Errors

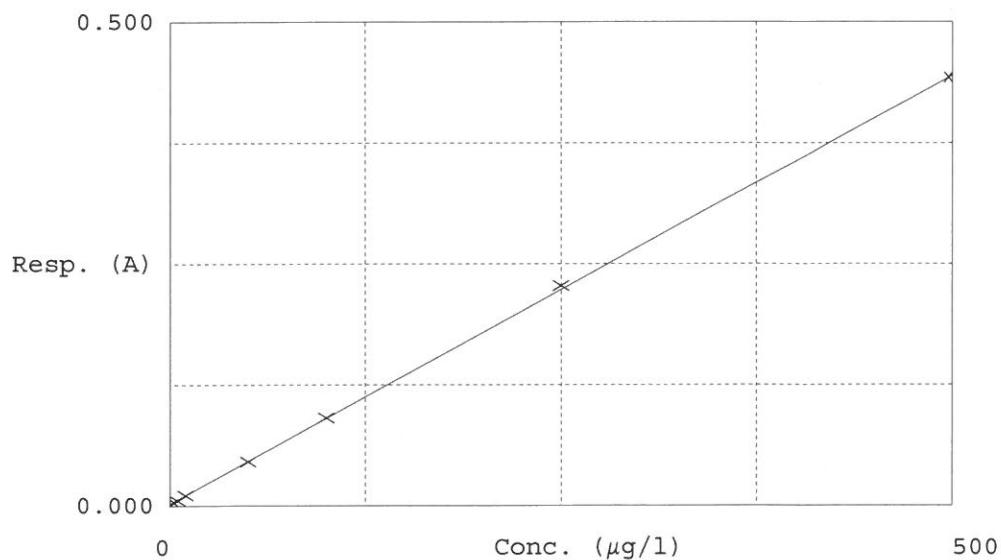

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.2441	0.0000	
2	5.0PPBCN	0.005	3.5890	5.0000	
3	10PPBCN	0.011	9.8897	10.0000	
4	50PPBCN	0.046	49.2409	50.0000	
5	100PPBCN	0.091	100.2388	100.0000	
6	250PPBCN	0.227	254.4825	250.0000	
7	500PPBCN	0.443	497.8032	500.0000	