

CB106218

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AL

Instrument ID : Konelab

11/12/2019 12:31

Test: ^{Reactive}~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.116	0.0	0.085	
ICB1	-0.460	0.0	0.001	
CCV1	245.353	0.0	0.215	
CCB1	-0.213	0.0	0.002	
PB124725BL	-0.253	0.0	0.001	
K5670-04	-0.531	0.0	0.001	
K5670-04DUP	-0.429	0.0	0.001	
K5788-06	-0.470	0.0	0.001	
K5789-04	-0.507	0.0	0.001	
K5789-08	-0.147	0.0	0.002	
K5789-12	-0.583	0.0	0.001	
CCV2	259.082	0.0	0.227	
CCB2	0.301	0.0	0.002	

N	13
Mean	45.943
SD	95.3597
CV%	207.56

AP

Aquakem v. 7.2AQ1

Results from time period:

Tue Nov 12 11:30:05 2019

Tue Nov 12 12:15:09 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	CI P	-0.2627	µg/l	11/12/2019 11:30:05	
5.OPPBCN	A	Reactive	CI P	4.6752	µg/l	11/12/2019 11:30:06	
10PPBCN	A	Reactive	CI P	9.2239	µg/l	11/12/2019 11:30:07	
50PPBCN	A	Reactive	CI P	49.5192	µg/l	11/12/2019 11:30:08	
100PPBCN	A	Reactive	CI P	100.427	µg/l	11/12/2019 11:30:09	
250PPBCN	A	Reactive	CI P	252.8718	µg/l	11/12/2019 11:30:10	
500PPBCN	A	Reactive	CI P	498.5456	µg/l	11/12/2019 11:30:11	
ICV1	S	Reactive	CI P	96.1159	µg/l	11/12/2019 12:11:45	
ICB1	S	Reactive	CI P	-0.4598	µg/l	11/12/2019 12:11:46	
CCV1	S	Reactive	CI P	245.3531	µg/l	11/12/2019 12:11:47	
CCB1	S	Reactive	CI P	-0.2131	µg/l	11/12/2019 12:11:48	
PB124725BL	S	Reactive	CI P	-0.2527	µg/l	11/12/2019 12:11:49	
K5670-04	S	Reactive	CI P	-0.5306	µg/l	11/12/2019 12:11:50	
K5670-04DUP	S	Reactive	CI P	-0.4291	µg/l	11/12/2019 12:11:51	
K5788-06	S	Reactive	CI P	-0.4697	µg/l	11/12/2019 12:11:52	
K5789-04	S	Reactive	CI P	-0.5066	µg/l	11/12/2019 12:11:53	
K5789-08	S	Reactive	CI P	-0.1469	µg/l	11/12/2019 12:11:54	
K5789-12	S	Reactive	CI P	-0.5833	µg/l	11/12/2019 12:11:55	
CCV2	S	Reactive	CI P	259.082	µg/l	11/12/2019 12:15:08	
CCB2	S	Reactive	CI P	0.3008	µg/l	11/12/2019 12:15:09	

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

Instrument ID : Konelab

11/12/2019 11:47


Test Total CN

Accepted 11/12/2019 11:47

Factor 1152
Bias 0.002

Coeff. of det. 0.999944

Errors

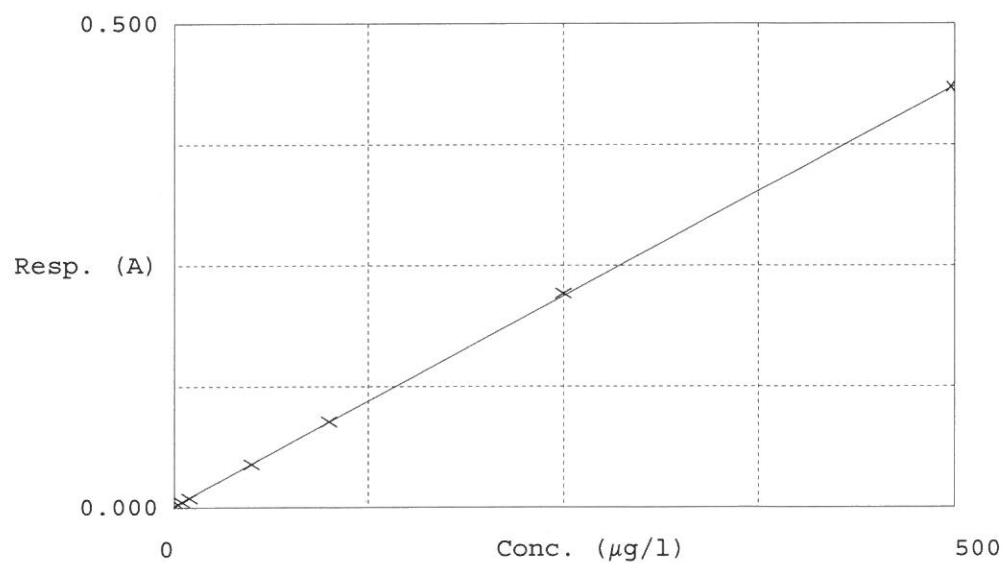

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.2627	0.0000	
2	5.0PPBCN	0.006	4.6752	5.0000	
3	10PPBCN	0.010	9.2239	10.0000	
4	50PPBCN	0.045	49.5192	50.0000	
5	100PPBCN	0.089	100.4270	100.0000	
6	250PPBCN	0.221	252.8718	250.0000	
7	500PPBCN	0.435	498.5456	500.0000	