

LB106228

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AL

Instrument ID : Konelab

11/12/2019 16:06

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.104	0.0	0.086	
ICB1	0.477	0.0	0.002	
CCV1	247.932	0.0	0.217	
CCB1	0.262	0.0	0.002	
PB124731BL	0.076	0.0	0.002	
PB124731BS	98.113	0.0	0.087	
MIDPB124731	248.624	0.0	0.218	
K5732-01	0.183	0.0	0.002	
K5732-01DUP	0.267	0.0	0.002	
K5732-01MS	42.743	0.0	0.039	
K5732-01MSD	42.295	0.0	0.038	
CCV2	262.054	0.0	0.229	
CCB2	-0.320	0.0	0.001	

N	13
Mean	79.985
SD	104.6656
CV%	130.86

Aquakem v. 7.2AQ1

AL

Results from time period:

Tue Nov 12 15:29:09 2019

Tue Nov 12 16:03:46 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.2627	µg/l	11/12/2019 11:30:05	
5.0PPBCN	A	Total CN	P	4.6752	µg/l	11/12/2019 11:30:06	
10PPBCN	A	Total CN	P	9.2239	µg/l	11/12/2019 11:30:07	
50PPBCN	A	Total CN	P	49.5192	µg/l	11/12/2019 11:30:08	
100PPBCN	A	Total CN	P	100.427	µg/l	11/12/2019 11:30:09	
250PPBCN	A	Total CN	P	252.8718	µg/l	11/12/2019 11:30:10	
500PPBCN	A	Total CN	P	498.5456	µg/l	11/12/2019 11:30:11	
ICV1	S	Total CN	P	97.1042	µg/l	11/12/2019 15:29:09	
ICB1	S	Total CN	P	0.4768	µg/l	11/12/2019 15:29:10	
CCV1	S	Total CN	P	247.932	µg/l	11/12/2019 15:29:11	
CCB1	S	Total CN	P	0.2621	µg/l	11/12/2019 15:29:12	
PB124731BL	S	Total CN	P	0.076	µg/l	11/12/2019 15:29:13	
PB124731BS	S	Total CN	P	98.1126	µg/l	11/12/2019 15:29:14	
MIDPB124731	S	Total CN	P	248.6243	µg/l	11/12/2019 15:29:19	
K5732-01	S	Total CN	P	0.1834	µg/l	11/12/2019 16:03:41	
K5732-01DUP	S	Total CN	P	0.2674	µg/l	11/12/2019 16:03:42	
K5732-01MS	S	Total CN	P	42.7435	µg/l	11/12/2019 16:03:43	
K5732-01MSD	S	Total CN	P	42.2949	µg/l	11/12/2019 16:03:44	
CCV2	S	Total CN	P	262.0545	µg/l	11/12/2019 16:03:45	
CCB2	S	Total CN	P	-0.3203	µg/l	11/12/2019 16:03:46	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

11/12/2019 11:47


Test Total CN

Accepted 11/12/2019 11:47

Factor 1152
Bias 0.002

Coeff. of det. 0.999944

Errors

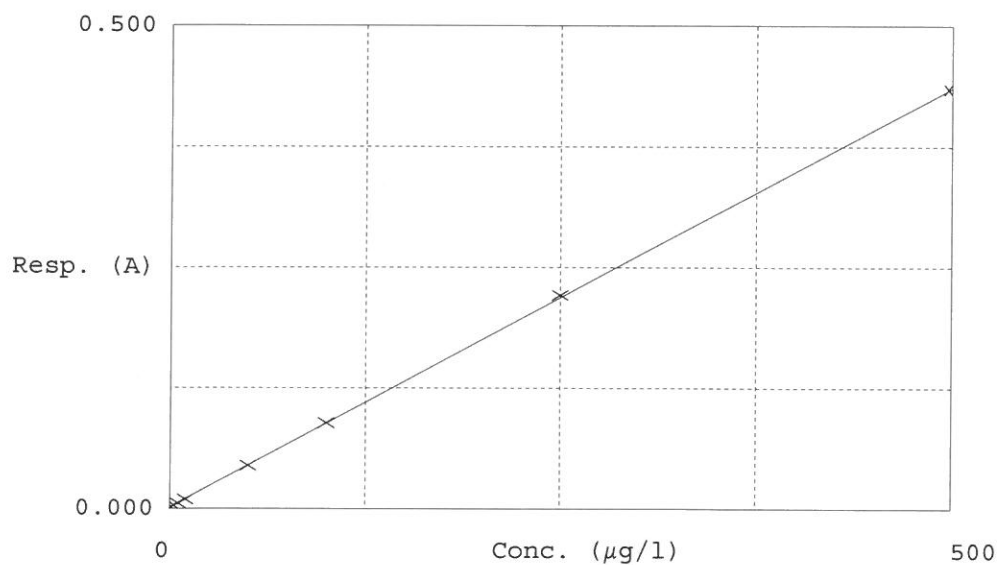

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.2627	0.0000	
2	5.0PPBCN	0.006	4.6752	5.0000	
3	10PPBCN	0.010	9.2239	10.0000	
4	50PPBCN	0.045	49.5192	50.0000	
5	100PPBCN	0.089	100.4270	100.0000	
6	250PPBCN	0.221	252.8718	250.0000	
7	500PPBCN	0.435	498.5456	500.0000	