

CB106322

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

11/15/2019 15:39

Test: *Reactive*
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.326	0.0	0.081	
ICB1	1.505	0.0	0.002	
CCV1	245.408	0.0	0.211	
CCB1	0.975	0.0	0.002	
PB124846BL	0.568	0.0	0.001	
K5782-08	0.892	0.0	0.002	
K5848-01	1.033	0.0	0.002	
K5862-04	0.461	0.0	0.001	
K5863-07	0.765	0.0	0.001	
K5864-02	0.923	0.0	0.002	
K5864-04	0.888	0.0	0.002	
CCV2	252.248	0.0	0.217	
CCB2	0.736	0.0	0.001	
K5864-06	0.701	0.0	0.001	
K5864-08	0.440	0.0	0.001	
K5864-10	0.743	0.0	0.001	
K5665-04	0.659	0.0	0.001	
K5665-04DUP	0.632	0.0	0.001	
K5671-10	0.678	0.0	0.001	
CCV3	261.780	0.0	0.225	
CCB3	1.253	0.0	0.002	

N	21
Mean	41.267
SD	90.9236
CV%	220.33

Aquakem v. 7.2AQ1

Results from time period:

Fri Nov 15 14:36:52 2019

Fri Nov 15 15:36:41 2019

Sample Id	Sam/Ctr/c/	Test short Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive Cl P	0.5131	µg/l	11/15/2019 14:36:52	
5.0PPBCN	A	Reactive Cl P	4.7542	µg/l	11/15/2019 14:36:53	
10PPBCN	A	Reactive Cl P	10.4265	µg/l	11/15/2019 14:36:54	
50PPBCN	A	Reactive Cl P	48.4189	µg/l	11/15/2019 14:36:55	
100PPBCN	A	Reactive Cl P	98.1701	µg/l	11/15/2019 14:36:56	
250PPBCN	A	Reactive Cl P	254.3984	µg/l	11/15/2019 14:36:57	
500PPBCN	A	Reactive Cl P	498.3188	µg/l	11/15/2019 14:36:58	
ICV1	S	Reactive Cl P	93.3258	µg/l	11/15/2019 15:12:21	
ICB1	S	Reactive Cl P	1.5045	µg/l	11/15/2019 15:12:22	
CCV1	S	Reactive Cl P	245.4082	µg/l	11/15/2019 15:12:23	
CCB1	S	Reactive Cl P	0.9749	µg/l	11/15/2019 15:12:24	
PB124846BL	S	Reactive Cl P	0.5678	µg/l	11/15/2019 15:12:25	
K5782-08	S	Reactive Cl P	0.8921	µg/l	11/15/2019 15:12:29	
K5848-01	S	Reactive Cl P	1.0333	µg/l	11/15/2019 15:12:30	
K5862-04	S	Reactive Cl P	0.4613	µg/l	11/15/2019 15:12:31	
K5863-07	S	Reactive Cl P	0.7652	µg/l	11/15/2019 15:19:28	
K5864-02	S	Reactive Cl P	0.9227	µg/l	11/15/2019 15:19:29	
K5864-04	S	Reactive Cl P	0.8877	µg/l	11/15/2019 15:19:30	
CCV2	S	Reactive Cl P	252.2482	µg/l	11/15/2019 15:19:31	
CCB2	S	Reactive Cl P	0.736	µg/l	11/15/2019 15:19:32	
K5864-06	S	Reactive Cl P	0.7009	µg/l	11/15/2019 15:19:33	
K5864-08	S	Reactive Cl P	0.4401	µg/l	11/15/2019 15:19:34	
K5864-10	S	Reactive Cl P	0.7434	µg/l	11/15/2019 15:19:35	
K5665-04	S	Reactive Cl P	0.6588	µg/l	11/15/2019 15:36:37	
K5665-04DUP	S	Reactive Cl P	0.6324	µg/l	11/15/2019 15:36:38	
K5671-10	S	Reactive Cl P	0.6784	µg/l	11/15/2019 15:36:39	
CCV3	S	Reactive Cl P	261.7795	µg/l	11/15/2019 15:36:40	
CCB3	S	Reactive Cl P	1.2535	µg/l	11/15/2019 15:36:41	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

11/15/2019 14:45


Test Total CN

Accepted 11/15/2019 14:45

Factor 1167
Bias 0.001

Coeff. of det. 0.999861

Errors

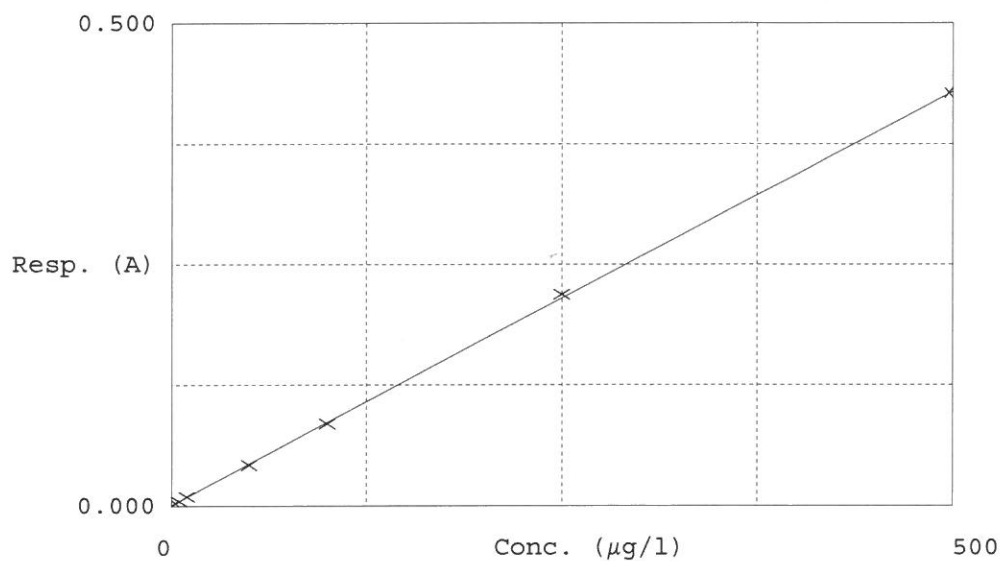

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.5131	0.0000	
2	5.0PPBCN	0.005	4.7542	5.0000	
3	10PPBCN	0.010	10.4265	10.0000	
4	50PPBCN	0.042	48.4189	50.0000	
5	100PPBCN	0.085	98.1701	100.0000	
6	250PPBCN	0.219	254.3984	250.0000	
7	500PPBCN	0.428	498.3188	500.0000	