

B106379

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AL

Instrument ID : Konelab

11/19/2019 10:47

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.143	0.0	0.104	
ICB1	-0.889	0.0	0.002	
CCV1	240.958	0.0	0.263	
CCB1	-0.974	0.0	0.001	
PB124897BL	-1.162	0.0	0.001	
K5669-08	-0.877	0.0	0.002	
K5669-08DUP	-0.886	0.0	0.002	
K5676-20	-0.880	0.0	0.002	
K5905-03	-0.892	0.0	0.002	
CCV2	242.948	0.0	0.265	
CCB2	-1.268	0.0	0.001	

N	11
Mean	51.838
SD	98.1815
CV%	189.40

Aquakem v. 7.2AQ1

Results from time period:

Tue Nov 19 08:58:40 2019



Tue Nov 19 10:20:24 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	Cl P	-0.6581	µg/l	11/19/2019 9:56:39	
5.OPPBCN	A	Reactive	Cl P	4.8623	µg/l	11/19/2019 9:56:40	
10PPBCN	A	Reactive	Cl P	10.2395	µg/l	11/19/2019 9:56:41	
50PPBCN	A	Reactive	Cl P	48.4724	µg/l	11/19/2019 9:56:42	
100PPBCN	A	Reactive	Cl P	99.7651	µg/l	11/19/2019 9:56:43	
250PPBCN	A	Reactive	Cl P	254.2448	µg/l	11/19/2019 9:56:44	
500PPBCN	A	Reactive	Cl P	498.0739	µg/l	11/19/2019 9:56:45	
ICV1	S	Reactive	Cl P	94.1427	µg/l	11/19/2019 10:20:14	
ICB1	S	Reactive	Cl P	-0.8887	µg/l	11/19/2019 10:20:15	
CCV1	S	Reactive	Cl P	240.9585	µg/l	11/19/2019 10:20:16	
CCB1	S	Reactive	Cl P	-0.9743	µg/l	11/19/2019 10:20:17	
PB124897BL	S	Reactive	Cl P	-1.1616	µg/l	11/19/2019 10:20:18	
K5669-08	S	Reactive	Cl P	-0.8769	µg/l	11/19/2019 10:20:19	
K5669-08DUP	S	Reactive	Cl P	-0.8863	µg/l	11/19/2019 10:20:20	
K5676-20	S	Reactive	Cl P	-0.88	µg/l	11/19/2019 10:20:21	
K5905-03	S	Reactive	Cl P	-0.892	µg/l	11/19/2019 10:20:22	
CCV2	S	Reactive	Cl P	242.948	µg/l	11/19/2019 10:20:23	
CCB2	S	Reactive	Cl P	-1.2683	µg/l	11/19/2019 10:20:24	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Ag

Instrument ID : Konelab

11/19/2019 9:58


Test Total CN

Accepted 11/19/2019 9:58

Factor 925.2
Bias 0.002

Coeff. of det. 0.999880

Errors

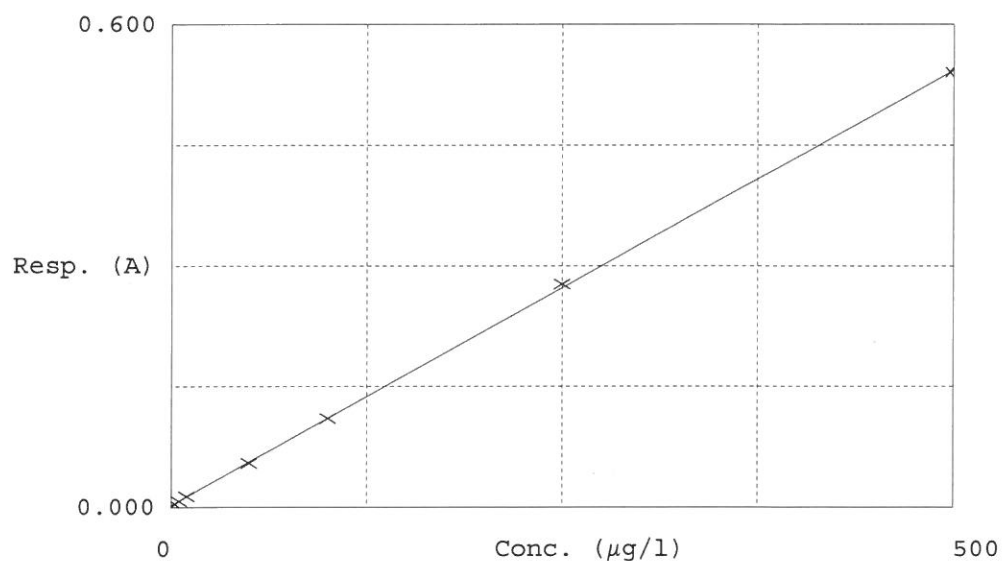

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.6581	0.0000	
2	5.0PPBCN	0.008	4.8623	5.0000	
3	10PPBCN	0.014	10.2395	10.0000	
4	50PPBCN	0.055	48.4724	50.0000	
5	100PPBCN	0.110	99.7651	100.0000	
6	250PPBCN	0.277	254.2448	250.0000	
7	500PPBCN	0.541	498.0739	500.0000	