

LB106485

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK Instrument ID : Konelab

11/26/2019 9:42

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.528	0.0	0.099	
ICB1	0.175	0.0	0.002	
CCV1	239.963	0.0	0.249	
CCB1	-0.013	0.0	0.002	
PB125066BL	0.025	0.0	0.002	
PB125066BS	95.238	0.0	0.100	
MIDPB125066	239.783	0.0	0.249	
K5960-07	5.323	0.0	0.007	
K5960-07DUP	5.374	0.0	0.007	
K5978-10	5.518	0.0	0.008	
CCV2	252.210	0.0	0.261	
CCB2	0.273	0.0	0.002	

N	12
Mean	78.200
SD	105.9155
CV%	135.44

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 25 17:36:07 2019

Mon Nov 25 18:03:57 2019

AK

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.0214	µg/l	11/25/2019 14:03:39	
5.0PPBCN	A	Total CN	P	5.2843	µg/l	11/25/2019 14:03:40	
10PPBCN	A	Total CN	P	10.5848	µg/l	11/25/2019 14:03:41	
50PPBCN	A	Total CN	P	50.4141	µg/l	11/25/2019 14:03:42	
100PPBCN	A	Total CN	P	99.4613	µg/l	11/25/2019 14:03:43	
250PPBCN	A	Total CN	P	248.4503	µg/l	11/25/2019 14:03:44	
500PPBCN	A	Total CN	P	500.8266	µg/l	11/25/2019 14:03:45	
ICV1	S	Total CN	P	94.5284	µg/l	11/25/2019 17:36:07	
ICB1	S	Total CN	P	0.1752	µg/l	11/25/2019 17:36:08	
CCV1	S	Total CN	P	239.9625	µg/l	11/25/2019 17:36:09	
CCB1	S	Total CN	P	-0.0134	µg/l	11/25/2019 17:36:10	
PB125066BL	S	Total CN	P	0.0249	µg/l	11/25/2019 17:36:11	
PB125066BS	S	Total CN	P	95.2377	µg/l	11/25/2019 17:36:12	
MIDPB125066	S	Total CN	P	239.7829	µg/l	11/25/2019 17:36:13	
K5960-07	S	Total CN	P	5.3229	µg/l	11/25/2019 18:03:53	
K5960-07DUP	S	Total CN	P	5.3745	µg/l	11/25/2019 18:03:54	
K5978-10	S	Total CN	P	5.5181	µg/l	11/25/2019 18:03:55	
CCV2	S	Total CN	P	252.2104	µg/l	11/25/2019 18:03:56	
CCB2	S	Total CN	P	0.2735	µg/l	11/25/2019 18:03:57	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

11/25/2019 14:06


Test Total CN

Accepted 11/25/2019 14:06

Factor 972.1
Bias 0.002

Coeff. of det. 0.999981

Errors

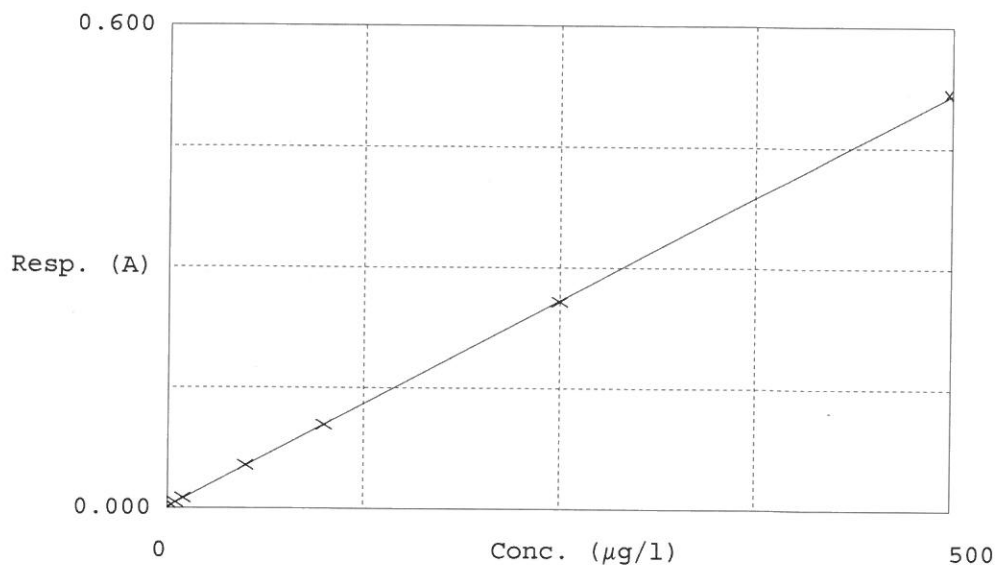

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.0214	0.0000	
2	5.0PPBCN	0.007	5.2843	5.0000	
3	10PPBCN	0.013	10.5848	10.0000	
4	50PPBCN	0.054	50.4141	50.0000	
5	100PPBCN	0.104	99.4613	100.0000	
6	250PPBCN	0.257	248.4503	250.0000	
7	500PPBCN	0.517	500.8266	500.0000	