

UB106527

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

11/27/2019 15:37

Test: Reactive
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	92.199	0.0	0.098	
ICB1	-0.083	0.0	0.002	
CCV1	248.810	0.0	0.262	
CCB1	-0.094	0.0	0.002	
PB125165BL	-0.318	0.0	0.002	
K5675-11	-0.261	0.0	0.002	
K5675-11DUP	-0.222	0.0	0.002	
K6054-03	-0.463	0.0	0.002	
K6054-06	-0.404	0.0	0.002	
K6066-04	-0.184	0.0	0.002	
CCV2	247.585	0.0	0.260	
CCB2	-0.427	0.0	0.002	

N 12
Mean 48.845
SD 96.8017
CV% 198.18

Aquakem v. 7.2AQ1

AE

Results from time period:

Wed Nov 27 15:34:19 2019

Wed Nov 27 15:37:07 2019

Sample Id	Sam/Ctr/c/	Test short Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive Cl P	-0.0545	µg/l	11/27/2019 14:18:21	
5.OPPBCN	A	Reactive Cl P	5.3857	µg/l	11/27/2019 14:18:22	
10PPBCN	A	Reactive Cl P	10.5943	µg/l	11/27/2019 14:18:23	
50PPBCN	A	Reactive Cl P	49.2904	µg/l	11/27/2019 14:18:24	
100PPBCN	A	Reactive Cl P	96.0211	µg/l	11/27/2019 14:18:25	
250PPBCN	A	Reactive Cl P	255.824	µg/l	11/27/2019 14:18:26	
500PPBCN	A	Reactive Cl P	497.9389	µg/l	11/27/2019 14:18:27	
ICV1	S	Reactive Cl P	92.199	µg/l	11/27/2019 15:34:19	
ICB1	S	Reactive Cl P	-0.0826	µg/l	11/27/2019 15:34:20	
CCV1	S	Reactive Cl P	248.81	µg/l	11/27/2019 15:34:21	
CCB1	S	Reactive Cl P	-0.0941	µg/l	11/27/2019 15:34:22	
PB125165BL	S	Reactive Cl P	-0.3181	µg/l	11/27/2019 15:34:23	
K5675-11	S	Reactive Cl P	-0.2612	µg/l	11/27/2019 15:34:24	
K5675-11DUP	S	Reactive Cl P	-0.2223	µg/l	11/27/2019 15:34:25	
K6054-03	S	Reactive Cl P	-0.4629	µg/l	11/27/2019 15:34:26	
K6054-06	S	Reactive Cl P	-0.404	µg/l	11/27/2019 15:34:27	
K6066-04	S	Reactive Cl P	-0.1839	µg/l	11/27/2019 15:34:28	
CCV2	S	Reactive Cl P	247.5846	µg/l	11/27/2019 15:34:29	
CCB2	S	Reactive Cl P	-0.4269	µg/l	11/27/2019 15:37:07	

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Ak Instrument ID : Konelab11/27/2019 14:25


Test Total CN

Accepted 11/27/2019 14:25

Factor 959
Bias 0.002

Coeff. of det. 0.999732

Errors

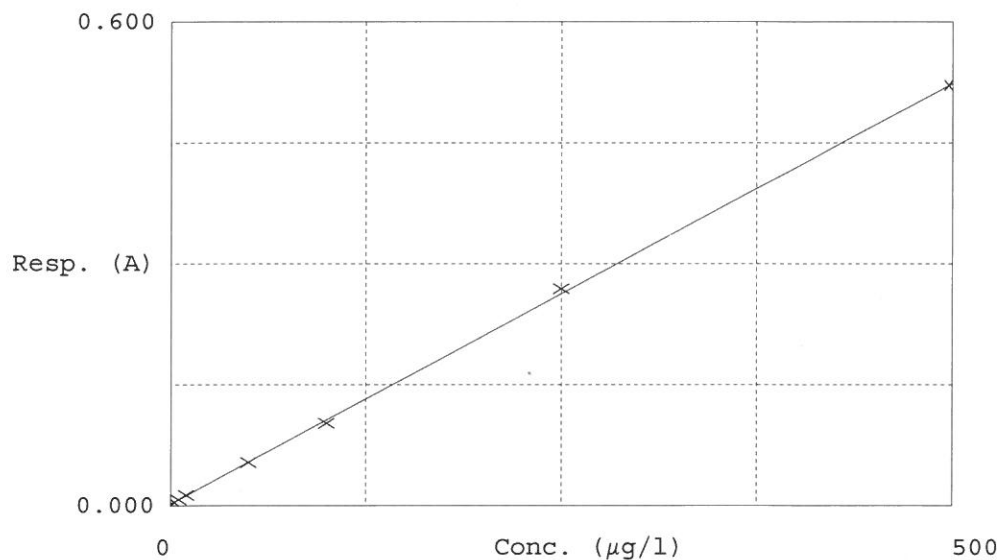

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.0545	0.0000	
2	5.0PPBCN	0.008	5.3857	5.0000	
3	10PPBCN	0.013	10.5943	10.0000	
4	50PPBCN	0.054	49.2904	50.0000	
5	100PPBCN	0.102	96.0211	100.0000	
6	250PPBCN	0.269	255.8240	250.0000	
7	500PPBCN	0.521	497.9389	500.0000	