


LB106561
INSTRUMENT ID CV1

7470A

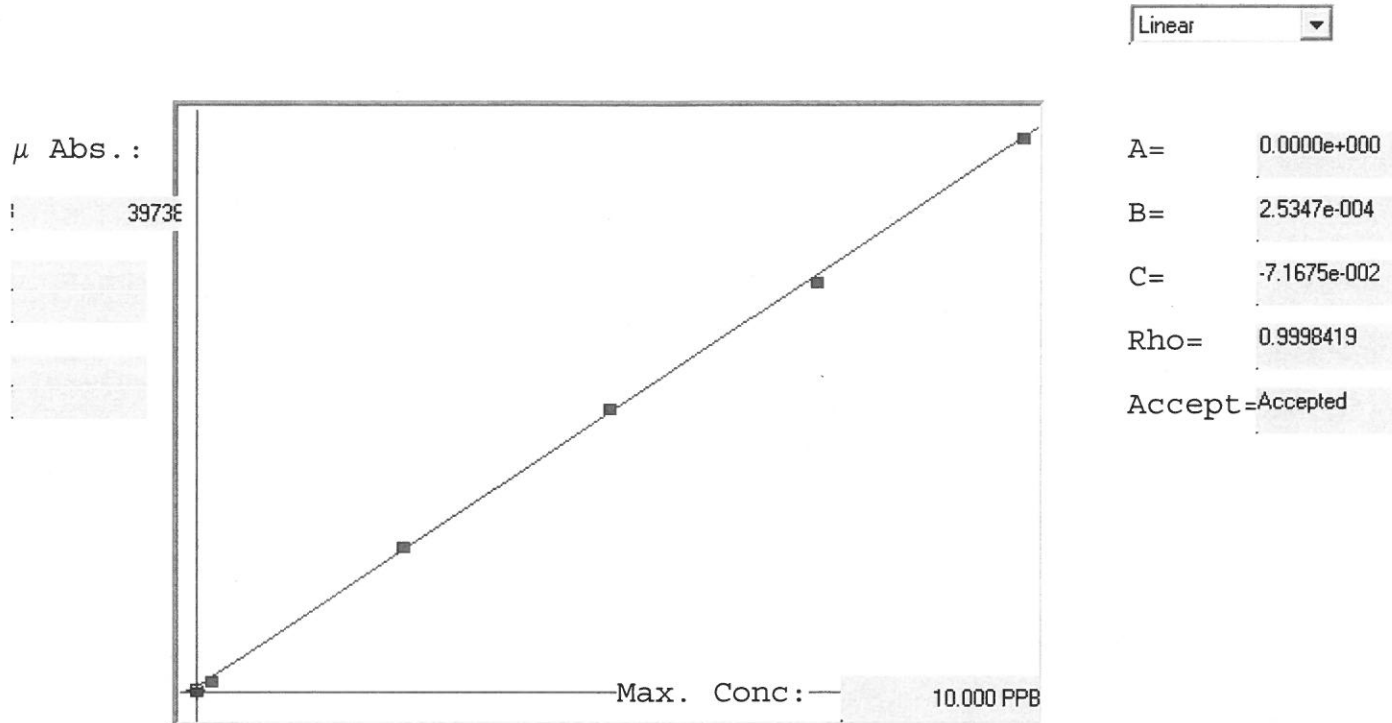

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.027	-0.027	176	0.000	176				
0.2	0.200	0.146	-0.054	857	0.0 %	857				
2.5	2.500	2.582	0.082	10469	0.0 %	10469				
5.0	5.000	5.087	0.087	20354	0.0 %	20354				
7.5	7.500	7.412	-0.088	29524	0.0 %	29524				
10.0	10.000	10.001	0.001	39738	0.0 %	39738				

LB106561 INSTRUMENT ID CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Dec 2019 13:55:06

Sample ID	Extended ID	µ Abs.	Conc.	Std CongMethod	Units	Date	Type	Type
0.0 - 1	50.0	176	-	0.00007470A	PPB	02 Dec 2019 14:00:23	S	Std
0.2 - 1	50.2	857	-	0.20007470A	PPB	02 Dec 2019 14:02:30	S	Std
2.5 - 1	52.6	10469	-	2.50007470A	PPB	02 Dec 2019 14:06:09	S	Std
5.0 - 1	55.0	20354	-	5.00007470A	PPB	02 Dec 2019 14:08:16	S	Std
7.5 - 1	57.6	29524	-	7.50007470A	PPB	02 Dec 2019 14:10:24	S	Std
10.0 - 1	510.0	39738	-	10.00007470A	PPB	02 Dec 2019 14:12:31	S	Std
ICV15 - 1	ICV15	16284	4.0558	-7470A	PPB	02 Dec 2019 14:15:04	U	SMPL
ICB15 - 1	ICB15	282	-0.0002	-7470A	PPB	02 Dec 2019 14:17:10	U	SMPL
CCV62 - 1	CCV62	20646	5.1614	-7470A	PPB	02 Dec 2019 14:19:16	U	SMPL
CCB62 - 1	CCB62	78	-0.0519	-7470A	PPB	02 Dec 2019 14:21:22	U	SMPL
CRA - 1	CRA	935	0.1653	-7470A	PPB	02 Dec 2019 14:23:29	U	SMPL
HighStd - 1	HighStd	39727	9.9978	-7470A	PPB	02 Dec 2019 14:25:35	U	SMPL
ChkStd - 1	ChkStd	27416	6.8774	-7470A	PPB	02 Dec 2019 14:27:41	U	SMPL
PB125219BL - 1	PBW	-32	-0.0798	-7470A	PPB	02 Dec 2019 14:29:48	U	SMPL
PB125219BS - 1	LCSW	15393	3.8299	-7470A	PPB	02 Dec 2019 14:31:52	U	SMPL
K6024-07 - 1	TWP-3	149	-0.0339	-7470A	PPB	02 Dec 2019 14:34:00	U	SMPL
K6024-07DUP - 1	TWP-3DUP	165	-0.0299	-7470A	PPB	02 Dec 2019 14:36:08	U	SMPL
K6024-07MS - 1	TWP-3MS	16769	4.1787	-7470A	PPB	02 Dec 2019 14:38:16	U	SMPL
K6024-07MSD - 1	TWP-3MSD	16883	4.2076	-7470A	PPB	02 Dec 2019 14:40:24	U	SMPL
K6024-08 - 1	TWP-6	154	-0.0326	-7470A	PPB	02 Dec 2019 14:42:31	U	SMPL
CCV63 - 1	CCV63	20240	5.0585	-7470A	PPB	02 Dec 2019 14:44:37	U	SMPL
CCB63 - 1	CCB63	131	-0.0385	-7470A	PPB	02 Dec 2019 14:46:43	U	SMPL
K6025-02 - 1	GROUNDWATER	180	-0.0261	-7470A	PPB	02 Dec 2019 14:48:49	U	SMPL
PB125220BL - 1	PBW	98	-0.0468	-7470A	PPB	02 Dec 2019 14:50:56	U	SMPL
PB125220BS - 1	LCSW	15458	3.8464	-7470A	PPB	02 Dec 2019 14:53:02	U	SMPL
K5676-38 - 1	SU-01-112719	116	-0.0423	-7470A	PPB	02 Dec 2019 14:55:09	U	SMPL
K5676-38DUP - 1	SU-01-112719DUP	133	-0.0380	-7470A	PPB	02 Dec 2019 14:57:15	U	SMPL
K5676-38MS - 1	SU-01-112719MS	16362	4.0755	-7470A	PPB	02 Dec 2019 14:59:23	U	SMPL
K5676-38MSD - 1	SU-01-112719MSD	16472	4.1034	-7470A	PPB	02 Dec 2019 15:01:30	U	SMPL
K6076-01 - 1	COMPOSITE-BIN-5-SOIL-PILE	107	-0.0446	-7470A	PPB	02 Dec 2019 15:03:38	U	SMPL
K6090-04 - 1	TP-20-S	126	-0.0397	-7470A	PPB	02 Dec 2019 15:05:46	U	SMPL
K6024-07LX5 - 1		40	-0.0615	-7470A	PPB	02 Dec 2019 15:07:52	U	SMPL
CCV64 - 1	CCV64	20007	4.9994	-7470A	PPB	02 Dec 2019 15:09:59	U	SMPL
CCB64 - 1	CCB64	109	-0.0440	-7470A	PPB	02 Dec 2019 15:12:05	U	SMPL
K5676-38LX5 - 1		28	-0.0646	-7470A	PPB	02 Dec 2019 15:14:12	U	SMPL
PB125220TB - 1	PB125179TB	140	-0.0362	-7470A	PPB	02 Dec 2019 15:16:18	U	SMPL
CCV65 - 1	CCV65	19533	4.8793	-7470A	PPB	02 Dec 2019 15:18:24	U	SMPL
CCB65 - 1	CCB65	120	-0.0413	-7470A	PPB	02 Dec 2019 15:20:30	U	SMPL