

LB1066 29

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AA

Instrument ID : Konelab

12/6/2019 10:52

Test: Reactive
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.699	0.0	0.110	
ICB1	0.120	0.0	0.003	
CCV1	240.213	0.0	0.273	
CCB1	-0.427	0.0	0.002	
PB125271BL	-0.325	0.0	0.002	
K6112-04	-0.174	0.0	0.002	
K6112-04DUP	0.124	0.0	0.003	
K6135-07	-0.294	0.0	0.002	
K6135-08	-0.189	0.0	0.002	
K6135-09	-0.522	0.0	0.002	
K6147-12	-0.102	0.0	0.002	
K6147-13	-0.249	0.0	0.002	
K6147-14	-0.119	0.0	0.002	
K6147-15	-0.032	0.0	0.002	
CCV2	243.919	0.0	0.277	
CCB2	-0.193	0.0	0.002	
K6147-16	-0.220	0.0	0.002	
K6147-17	-0.287	0.0	0.002	
K6147-18	0.161	0.0	0.003	
K6147-19	-0.232	0.0	0.002	
K6147-20	-0.270	0.0	0.002	
K6147-21	-0.197	0.0	0.002	
K6147-22	-0.432	0.0	0.002	
CCV3	257.458	0.0	0.292	
CCB3	0.021	0.0	0.002	

N	25
Mean	33.338
SD	82.8799
CV%	248.60

Aquakem v. 7.2AQ1

AK

Results from time period:

Fri Dec 06 10:11:10 2019

Fri Dec 06 10:51:35 2019

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.6774	µg/l	12/6/2019 10:11:10	
5.OPPBCN	A	Reactive CN	P	4.1606	µg/l	12/6/2019 10:11:11	
10PPBCN	A	Reactive CN	P	9.1626	µg/l	12/6/2019 10:11:12	
50PPBCN	A	Reactive CN	P	49.4944	µg/l	12/6/2019 10:11:13	
100PPBCN	A	Reactive CN	P	101.8458	µg/l	12/6/2019 10:11:14	
250PPBCN	A	Reactive CN	P	252.6148	µg/l	12/6/2019 10:11:15	
500PPBCN	A	Reactive CN	P	498.3992	µg/l	12/6/2019 10:11:16	
ICV1	S	Reactive CN	P	95.6986	µg/l	12/6/2019 10:40:07	
ICB1	S	Reactive CN	P	0.1204	µg/l	12/6/2019 10:40:08	
CCV1	S	Reactive CN	P	240.2134	µg/l	12/6/2019 10:40:09	
CCB1	S	Reactive CN	P	-0.4268	µg/l	12/6/2019 10:40:10	
PB125271BL	S	Reactive CN	P	-0.3248	µg/l	12/6/2019 10:40:11	
K6112-04	S	Reactive CN	P	-0.1744	µg/l	12/6/2019 10:40:12	
K6112-04DUP	S	Reactive CN	P	0.1239	µg/l	12/6/2019 10:40:13	
K6135-07	S	Reactive CN	P	-0.2942	µg/l	12/6/2019 10:40:14	
K6135-08	S	Reactive CN	P	-0.1894	µg/l	12/6/2019 10:40:15	
K6135-09	S	Reactive CN	P	-0.522	µg/l	12/6/2019 10:40:16	
K6147-12	S	Reactive CN	P	-0.1023	µg/l	12/6/2019 10:40:17	
K6147-13	S	Reactive CN	P	-0.2494	µg/l	12/6/2019 10:47:42	
K6147-14	S	Reactive CN	P	-0.1194	µg/l	12/6/2019 10:47:43	
K6147-15	S	Reactive CN	P	-0.0321	µg/l	12/6/2019 10:47:44	
CCV2	S	Reactive CN	P	243.9194	µg/l	12/6/2019 10:47:45	
CCB2	S	Reactive CN	P	-0.1925	µg/l	12/6/2019 10:47:46	
K6147-16	S	Reactive CN	P	-0.2203	µg/l	12/6/2019 10:47:47	
K6147-17	S	Reactive CN	P	-0.2872	µg/l	12/6/2019 10:47:48	
K6147-18	S	Reactive CN	P	0.1612	µg/l	12/6/2019 10:47:49	
K6147-19	S	Reactive CN	P	-0.2324	µg/l	12/6/2019 10:47:50	
K6147-20	S	Reactive CN	P	-0.2704	µg/l	12/6/2019 10:47:51	
K6147-21	S	Reactive CN	P	-0.1973	µg/l	12/6/2019 10:47:52	
K6147-22	S	Reactive CN	P	-0.432	µg/l	12/6/2019 10:51:33	
CCV3	S	Reactive CN	P	257.4579	µg/l	12/6/2019 10:51:34	
CCB3	S	Reactive CN	P	0.0215	µg/l	12/6/2019 10:51:35	

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

12/6/2019 10:12


Test Total CN

Accepted 12/6/2019 10:12

Factor 888.3
Bias 0.002

Coeff. of det. 0.999927

Errors

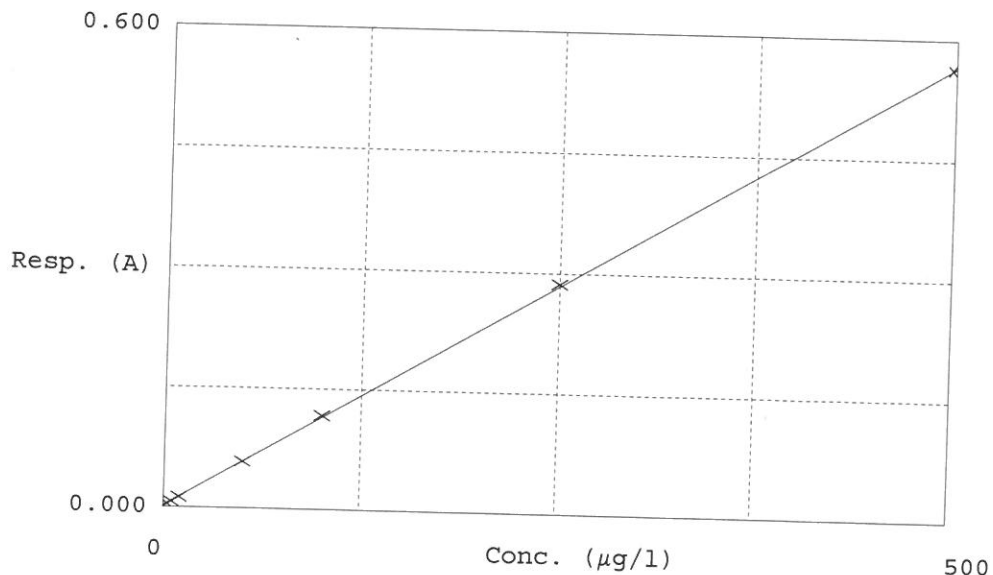

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.6774	0.0000	
2	5.0PPBCN	0.007	4.1606	5.0000	
3	10PPBCN	0.013	9.1626	10.0000	
4	50PPBCN	0.058	49.4944	50.0000	
5	100PPBCN	0.117	101.8458	100.0000	
6	250PPBCN	0.287	252.6148	250.0000	
7	500PPBCN	0.563	498.3992	500.0000	