


LB106678
INSTRUMENT ID CU1

245.1

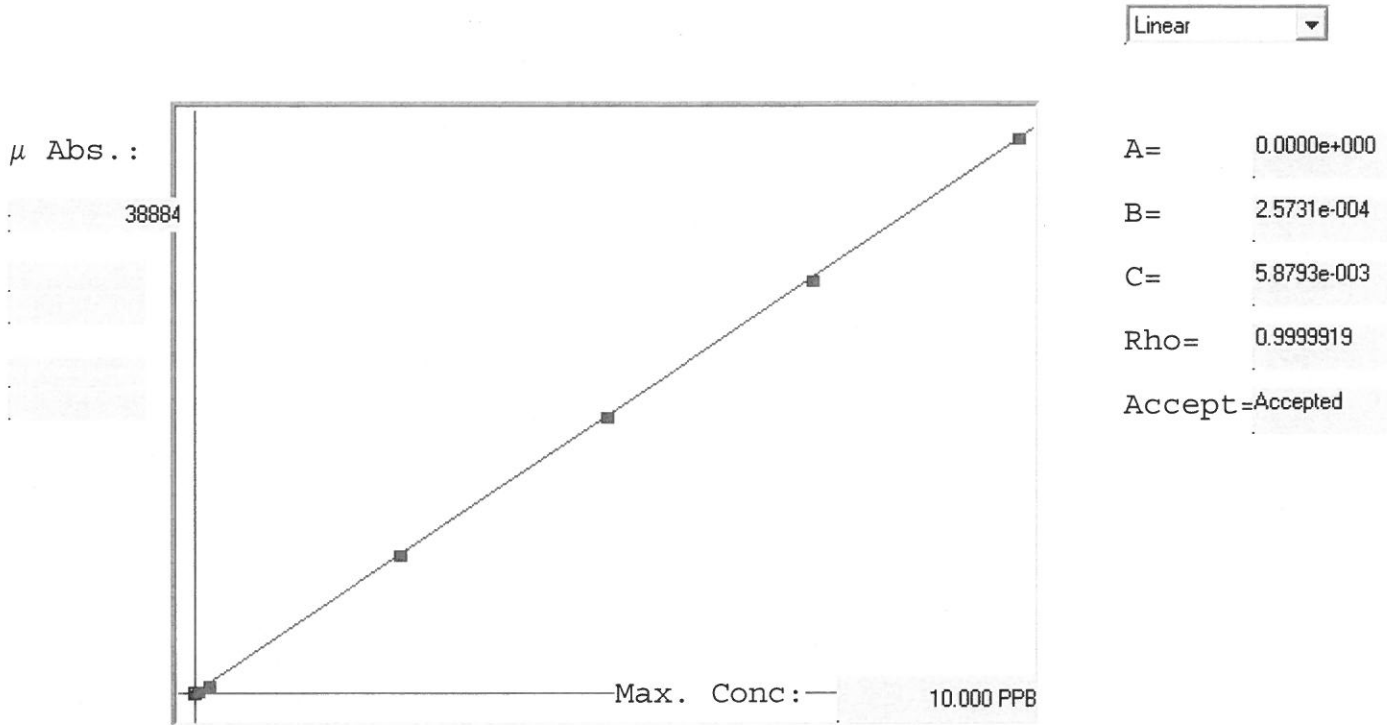

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.013	0.013	29	0.000	29				
0.05	0.050	0.056	0.006	193	0.0 %	193				
0.2	0.200	0.177	-0.023	664	0.0 %	664				
2.5	2.500	2.507	0.007	9720	0.0 %	9720				
5.0	5.000	5.009	0.009	19445	0.0 %	19445				
7.5	7.500	7.477	-0.023	29034	0.0 %	29034				
10.0	10.000	10.011	0.011	38884	0.0 %	38884				

LB106678 INSTRUMENT ID CV1

Method: 245.1

Operator: Admin

Date of Analysis: 11 Dec 2019 08:04:17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	29	-	0.0000	245.1	PPB	11 Dec 2019 08:09:43	S	Std
0.05 - 1	50.05	193	-	0.0500	245.1	PPB	11 Dec 2019 08:12:00	S	Std
0.2 - 1	50.2	664	-	0.2000	245.1	PPB	11 Dec 2019 08:14:17	S	Std
2.5 - 1	52.5	9720	-	2.5000	245.1	PPB	11 Dec 2019 08:16:34	S	Std
5.0 - 1	55.0	19445	-	5.0000	245.1	PPB	11 Dec 2019 08:18:51	S	Std
7.5 - 1	57.5	29034	-	7.5000	245.1	PPB	11 Dec 2019 08:23:44	S	Std
10.0 - 1	510.0	38884	-	10.0000	245.1	PPB	11 Dec 2019 08:27:39	S	Std
ICV22 - 1	ICV22	14776	3.8080	-245.1		PPB	11 Dec 2019 08:31:08	U	SMPL
ICB22 - 1	ICB22	12	0.0090	-245.1		PPB	11 Dec 2019 08:33:24	U	SMPL
CCV94 - 1	CCV94	18960	4.8846	-245.1		PPB	11 Dec 2019 08:35:39	U	SMPL
CCB94 - 1	CCB94	8	0.0079	-245.1		PPB	11 Dec 2019 08:37:55	U	SMPL
CRA - 1	CRA	196	0.0563	-245.1		PPB	11 Dec 2019 08:47:21	U	SMPL
HighStd - 1	HighStd	38232	9.8435	-245.1		PPB	11 Dec 2019 08:49:36	U	SMPL
ChkStd - 1	ChkStd	26010	6.6986	-245.1		PPB	11 Dec 2019 08:51:51	U	SMPL
PB125357BL - 1	PBW	-3	0.0051	-245.1		PPB	11 Dec 2019 08:54:08	U	SMPL
PB125357BS - 1	LCSW	15135	3.9003	-245.1		PPB	11 Dec 2019 08:56:24	U	SMPL
K6131-02 - 1	COMP	163	0.0478	-245.1		PPB	11 Dec 2019 09:06:34	U	SMPL
K6131-02DUP - 1	COMP DUP	163	0.0478	-245.1		PPB	11 Dec 2019 09:08:50	U	SMPL
K6131-02MS - 1	COMPMS	13369	3.4459	-245.1		PPB	11 Dec 2019 09:11:07	U	SMPL
K6131-02MSD - 1	COMPMSD	13525	3.4861	-245.1		PPB	11 Dec 2019 09:13:24	U	SMPL
K6217-01 - 1	TI-633-EB	80	0.0265	-245.1		PPB	11 Dec 2019 09:15:40	U	SMPL
CCV95 - 1	CCV95	18947	4.8812	-245.1		PPB	11 Dec 2019 09:17:57	U	SMPL
CCB95 - 1	CCB95	77	0.0257	-245.1		PPB	11 Dec 2019 09:20:12	U	SMPL
K6217-03 - 1	TI-633	158	0.0465	-245.1		PPB	11 Dec 2019 09:22:27	U	SMPL
K6217-04 - 1	TI-633-X	149	0.0442	-245.1		PPB	11 Dec 2019 09:24:43	U	SMPL
K6218-02 - 1	TI-604	316	0.0872	-245.1		PPB	11 Dec 2019 09:26:58	U	SMPL
K6229-01 - 1	391204857.0	244	0.0687	-245.1		PPB	11 Dec 2019 09:29:14	U	SMPL
K6230-01 - 1	391204847.0	170	0.0496	-245.1		PPB	11 Dec 2019 09:31:30	U	SMPL
K6231-01 - 1	391204031.0	70	0.0239	-245.1		PPB	11 Dec 2019 09:33:46	U	SMPL
K6232-01 - 1	391203045.1	108	0.0337	-245.1		PPB	11 Dec 2019 09:36:03	U	SMPL
K6233-01 - 1	391205018.0	116	0.0357	-245.1		PPB	11 Dec 2019 09:38:20	U	SMPL
K6131-02LX5 - 1		10	0.0085	-245.1		PPB	11 Dec 2019 09:40:38	U	SMPL
K6131-02A - 1		15442	3.9793	-245.1		PPB	11 Dec 2019 09:42:52	U	SMPL
CCV96 - 1	CCV96	19261	4.9620	-245.1		PPB	11 Dec 2019 09:51:10	U	SMPL
CCB96 - 1	CCB96	17	0.0103	-245.1		PPB	11 Dec 2019 09:53:26	U	SMPL