

CB106769

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

12/16/2019 10:32

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.980	0.0	0.094	
ICB1	-0.344	0.0	0.002	
CCV1	244.941	0.0	0.235	
CCB1	-0.244	0.0	0.002	
PB125457BL	-0.494	0.0	0.002	
K6110-04	-0.483	0.0	0.002	
K6110-04DUP	-0.444	0.0	0.002	
K6265-04	-0.574	0.0	0.001	
K6265-08	-0.540	0.0	0.001	
K6274-03	-0.392	0.0	0.002	
PB125459BL	-0.582	0.0	0.001	
K6283-02	-0.567	0.0	0.001	
K6283-02DUP	-0.455	0.0	0.002	
K6283-01	-0.590	0.0	0.001	
CCV2	262.336	0.0	0.252	
CCB2	-0.506	0.0	0.002	

N	16
Mean	37.378
SD	87.8904
CV%	235.14

Aquakem v. 7.2AQ1

Results from time period:

Mon Dec 16 09:31:11 2019

AC

Mon Dec 16 10:28:38 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	Cl P	-0.2419	µg/l	12/16/2019 9:31:11	
5.OPPBCN	A	Reactive	Cl P	4.5988	µg/l	12/16/2019 9:31:12	
10PPBCN	A	Reactive	Cl P	9.5286	µg/l	12/16/2019 9:31:13	
50PPBCN	A	Reactive	Cl P	49.9715	µg/l	12/16/2019 9:31:14	
100PPBCN	A	Reactive	Cl P	100.2586	µg/l	12/16/2019 9:31:15	
250PPBCN	A	Reactive	Cl P	251.8398	µg/l	12/16/2019 9:31:16	
500PPBCN	A	Reactive	Cl P	499.0446	µg/l	12/16/2019 9:31:17	
ICV1	S	Reactive	Cl P	96.9803	µg/l	12/16/2019 10:04:13	
ICB1	S	Reactive	Cl P	-0.3439	µg/l	12/16/2019 10:04:14	
CCV1	S	Reactive	Cl P	244.9409	µg/l	12/16/2019 10:04:15	
CCB1	S	Reactive	Cl P	-0.2436	µg/l	12/16/2019 10:04:16	
PB125457BL	S	Reactive	Cl P	-0.4937	µg/l	12/16/2019 10:04:17	
K6110-04	S	Reactive	Cl P	-0.4835	µg/l	12/16/2019 10:04:18	
K6110-04DUP	S	Reactive	Cl P	-0.4442	µg/l	12/16/2019 10:04:19	
K6265-04	S	Reactive	Cl P	-0.5745	µg/l	12/16/2019 10:04:20	
K6265-08	S	Reactive	Cl P	-0.5397	µg/l	12/16/2019 10:04:21	
K6274-03	S	Reactive	Cl P	-0.3916	µg/l	12/16/2019 10:04:22	
PB125459BL	S	Reactive	Cl P	-0.582	µg/l	12/16/2019 10:09:00	
K6283-02	S	Reactive	Cl P	-0.5672	µg/l	12/16/2019 10:09:01	
K6283-02DUP	S	Reactive	Cl P	-0.4553	µg/l	12/16/2019 10:09:02	
K6283-01	S	Reactive	Cl P	-0.5895	µg/l	12/16/2019 10:28:36	
CCV2	S	Reactive	Cl P	262.3355	µg/l	12/16/2019 10:28:37	
CCB2	S	Reactive	Cl P	-0.5057	µg/l	12/16/2019 10:28:38	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AR

Instrument ID : Konelab

12/16/2019 9:34


Test Total CN

Accepted 12/16/2019 9:34

Factor 1049
Bias 0.002

Coeff. of det. 0.999977

Errors

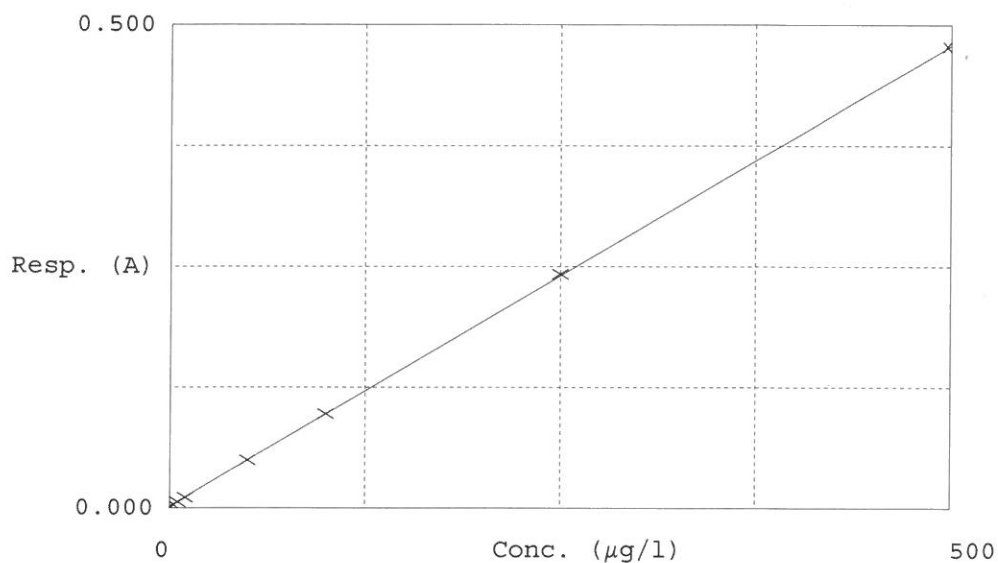

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.2419	0.0000	
2	5.0PPBCN	0.006	4.5988	5.0000	
3	10PPBCN	0.011	9.5286	10.0000	
4	50PPBCN	0.050	49.9715	50.0000	
5	100PPBCN	0.098	100.2586	100.0000	
6	250PPBCN	0.242	251.8398	250.0000	
7	500PPBCN	0.478	499.0446	500.0000	