

68106790

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Ad

Instrument ID : Konelab

12/17/2019 11:01

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.917	0.0	0.096	
ICB1	0.551	0.0	0.002	
CCV1	240.163	0.0	0.239	
CCB1	0.486	0.0	0.002	
PB125507BL	0.455	0.0	0.002	
PB125507BS	96.037	0.0	0.096	
MIDPB125507	242.480	0.0	0.241	
K6312-07	0.821	0.0	0.002	
K6312-07DUP	0.645	0.0	0.002	
K6321-01	0.878	0.0	0.002	
K6312-07MS	41.019	0.0	0.042	
K6312-07MSD	42.172	0.0	0.043	
CCV2	256.227	0.0	0.255	
CCB2	0.462	0.0	0.002	

N	14
Mean	72.737
SD	99.9790
CV%	137.45

Aquakem v. 7.2AQ1

Results from time period:

Tue Dec 17 10:04:04 2019

Tue Dec 17 10:57:48 2019

FA

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.2105	µg/l	12/17/2019 10:04:04	
5.OPPBCN	A	Total CN	P	5.213	µg/l	12/17/2019 10:04:05	
10PPBCN	A	Total CN	P	10.3083	µg/l	12/17/2019 10:04:06	
50PPBCN	A	Total CN	P	49.2089	µg/l	12/17/2019 10:04:07	
100PPBCN	A	Total CN	P	100.7115	µg/l	12/17/2019 10:04:08	
250PPBCN	A	Total CN	P	248.8385	µg/l	12/17/2019 10:04:09	
500PPBCN	A	Total CN	P	500.5093	µg/l	12/17/2019 10:04:10	
ICV1	S	Total CN	P	95.9169	µg/l	12/17/2019 10:30:34	
ICB1	S	Total CN	P	0.5509	µg/l	12/17/2019 10:30:35	
CCV1	S	Total CN	P	240.1631	µg/l	12/17/2019 10:30:36	
CCB1	S	Total CN	P	0.4862	µg/l	12/17/2019 10:30:37	
PB125507BL	S	Total CN	P	0.4553	µg/l	12/17/2019 10:30:38	
PB125507BS	S	Total CN	P	96.0369	µg/l	12/17/2019 10:30:39	
MIDPB125507	S	Total CN	P	242.4795	µg/l	12/17/2019 10:30:40	
K6312-07	S	Total CN	P	0.8207	µg/l	12/17/2019 10:30:41	
K6312-07DUP	S	Total CN	P	0.6451	µg/l	12/17/2019 10:30:42	
K6321-01	S	Total CN	P	0.8782	µg/l	12/17/2019 10:34:25	
K6312-07MS	S	Total CN	P	41.0194	µg/l	12/17/2019 10:57:45	
K6312-07MSD	S	Total CN	P	42.1717	µg/l	12/17/2019 10:57:46	
CCV2	S	Total CN	P	256.227	µg/l	12/17/2019 10:57:47	
CCB2	S	Total CN	P	0.4617	µg/l	12/17/2019 10:57:48	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

12/17/2019 10:05


Test Total CN

Accepted 12/17/2019 10:05

Factor 1012
Bias 0.001

Coeff. of det. 0.999986

Errors

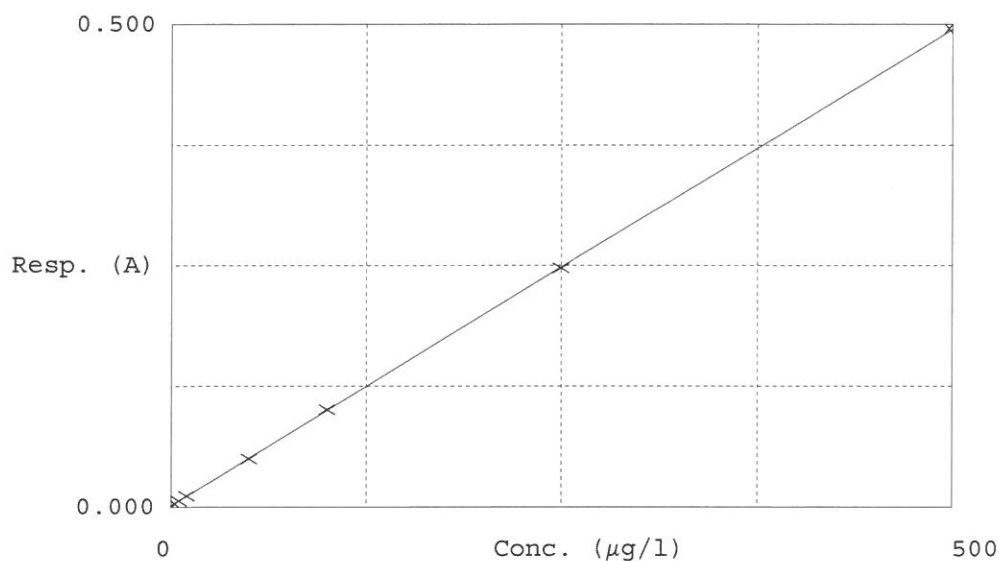

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.2105	0.0000	
2	5.0PPBCN	0.007	5.2130	5.0000	
3	10PPBCN	0.012	10.3083	10.0000	
4	50PPBCN	0.050	49.2089	50.0000	
5	100PPBCN	0.101	100.7115	100.0000	
6	250PPBCN	0.247	248.8385	250.0000	
7	500PPBCN	0.496	500.5093	500.0000	