

LB106797

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Alu

Instrument ID : Konelab

12/17/2019 12:04

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.310	0.0	0.096	
ICB1	0.495	0.0	0.002	
CCV1	242.206	0.0	0.241	
CCB1	0.486	0.0	0.002	
PB125458BL	0.483	0.0	0.002	
PB125458BS	98.128	0.0	0.098	
LOWPB125458	10.498	0.0	0.012	
HIGHPB125458	491.824	0.0	0.487	
K6112-05	1.408	0.0	0.003	
K6112-05DUP	1.233	0.0	0.003	
K6112-05MS	28.694	0.0	0.030	
K6112-05MSD	28.009	0.0	0.029	
K6113-06	0.661	0.0	0.002	
K6117-04	0.576	0.0	0.002	
CCV2	239.601	0.0	0.238	
CCB2	0.372	0.0	0.002	
K6118-06	0.255	0.0	0.002	
K6292-01	1.905	0.0	0.003	
K6294-01	0.429	0.0	0.002	
K6294-04	0.611	0.0	0.002	
K6310-03	2.359	0.0	0.004	
K6317-07	0.478	0.0	0.002	
K6317-08	0.167	0.0	0.002	
CCV3	258.180	0.0	0.257	
CCB3	0.416	0.0	0.002	

N	25
Mean	60.191
SD	121.5339
CV%	201.91

Aquakem v. 7.2AQ1

AK

Results from time period:

Tue Dec 17 11:38:42 2019

Tue Dec 17 11:50:10 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.2105	µg/l	12/17/2019 10:04:04	
5.OPPBCN	A	Total CN	P	5.213	µg/l	12/17/2019 10:04:05	
10PPBCN	A	Total CN	P	10.3083	µg/l	12/17/2019 10:04:06	
50PPBCN	A	Total CN	P	49.2089	µg/l	12/17/2019 10:04:07	
100PPBCN	A	Total CN	P	100.7115	µg/l	12/17/2019 10:04:08	
250PPBCN	A	Total CN	P	248.8385	µg/l	12/17/2019 10:04:09	
500PPBCN	A	Total CN	P	500.5093	µg/l	12/17/2019 10:04:10	
ICV1	S	Total CN	P	95.3099	µg/l	12/17/2019 11:38:42	
ICB1	S	Total CN	P	0.4946	µg/l	12/17/2019 11:38:43	
CCV1	S	Total CN	P	242.2058	µg/l	12/17/2019 11:38:44	
CCB1	S	Total CN	P	0.4859	µg/l	12/17/2019 11:38:45	
PB125458BL	S	Total CN	P	0.4834	µg/l	12/17/2019 11:38:46	
PB125458BS	S	Total CN	P	98.1277	µg/l	12/17/2019 11:38:47	
LOWPB125458	S	Total CN	P	10.4979	µg/l	12/17/2019 11:38:48	
HIGHPB125458	S	Total CN	P	491.8239	µg/l	12/17/2019 11:38:49	
K6112-05	S	Total CN	P	1.4079	µg/l	12/17/2019 11:38:50	
K6112-05DUP	S	Total CN	P	1.2328	µg/l	12/17/2019 11:38:51	
K6112-05MS	S	Total CN	P	28.6942	µg/l	12/17/2019 11:38:52	
K6112-05MSD	S	Total CN	P	28.0088	µg/l	12/17/2019 11:46:17	
K6113-06	S	Total CN	P	0.6606	µg/l	12/17/2019 11:46:18	
K6117-04	S	Total CN	P	0.5763	µg/l	12/17/2019 11:46:19	
CCV2	S	Total CN	P	239.6013	µg/l	12/17/2019 11:46:20	
CCB2	S	Total CN	P	0.3721	µg/l	12/17/2019 11:46:21	
K6118-06	S	Total CN	P	0.2552	µg/l	12/17/2019 11:46:22	
K6292-01	S	Total CN	P	1.9051	µg/l	12/17/2019 11:46:23	
K6294-01	S	Total CN	P	0.4287	µg/l	12/17/2019 11:46:24	
K6294-04	S	Total CN	P	0.6107	µg/l	12/17/2019 11:46:25	
K6310-03	S	Total CN	P	2.3588	µg/l	12/17/2019 11:46:26	
K6317-07	S	Total CN	P	0.4783	µg/l	12/17/2019 11:46:27	
K6317-08	S	Total CN	P	0.1673	µg/l	12/17/2019 11:50:08	
CCV3	S	Total CN	P	258.18	µg/l	12/17/2019 11:50:09	
CCB3	S	Total CN	P	0.4159	µg/l	12/17/2019 11:50:10	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : NE

Instrument ID : Konelab

12/17/2019 13:19


Test Total CN

Accepted 12/17/2019 10:05

Factor 1012
Bias 0.001

Coeff. of det. 0.999986

Errors

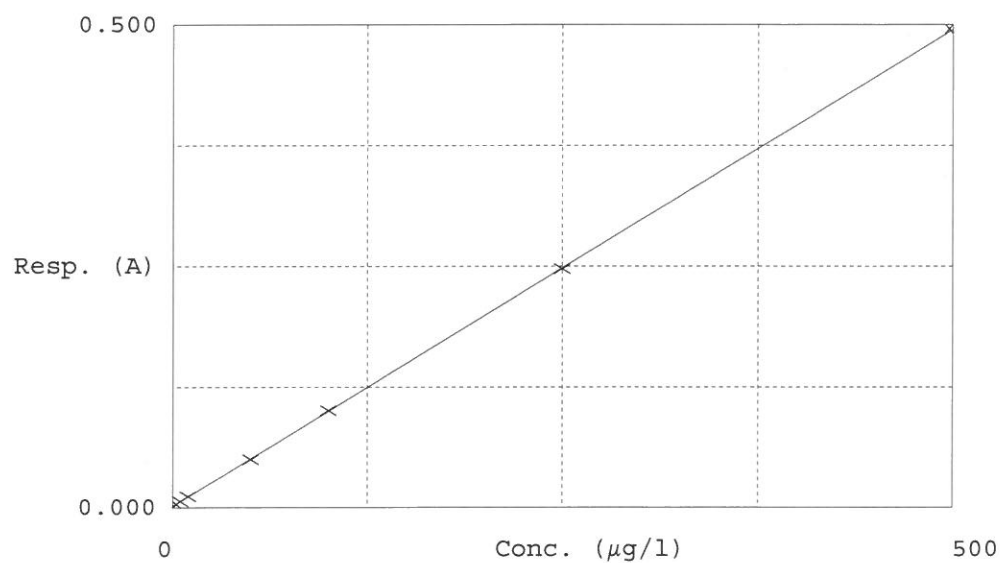

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.2105	0.0000	
2	5.0PPBCN	0.007	5.2130	5.0000	
3	10PPBCN	0.012	10.3083	10.0000	
4	50PPBCN	0.050	49.2089	50.0000	
5	100PPBCN	0.101	100.7115	100.0000	
6	250PPBCN	0.247	248.8385	250.0000	
7	500PPBCN	0.496	500.5093	500.0000	