

LB10683-8

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AR

Instrument ID : Konelab

12/18/2019 16:36

Test: ^{Reactive} Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.646	0.0	0.112	
ICB1	0.412	0.0	0.002	
CCV1	239.089	0.0	0.277	
CCB1	0.194	0.0	0.002	
PB125588BL	0.103	0.0	0.002	
K6310-04	-0.053	0.0	0.002	
K6359-03	-0.220	0.0	0.001	
K6359-03DUP	0.058	0.0	0.002	
K6359-04	-0.212	0.0	0.001	
K6359-05	0.192	0.0	0.002	
K6360-02	0.096	0.0	0.002	
CCV2	259.689	0.0	0.300	
CCB2	0.150	0.0	0.002	

N	13
Mean	45.780
SD	94.2093
CV%	205.79

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AD

Instrument ID : Konelab

12/18/2019 15:59

Test Total CN


Accepted 12/18/2019 15:59

Factor 869.9

Bias 0.002

Coeff. of det. 0.999951

Errors

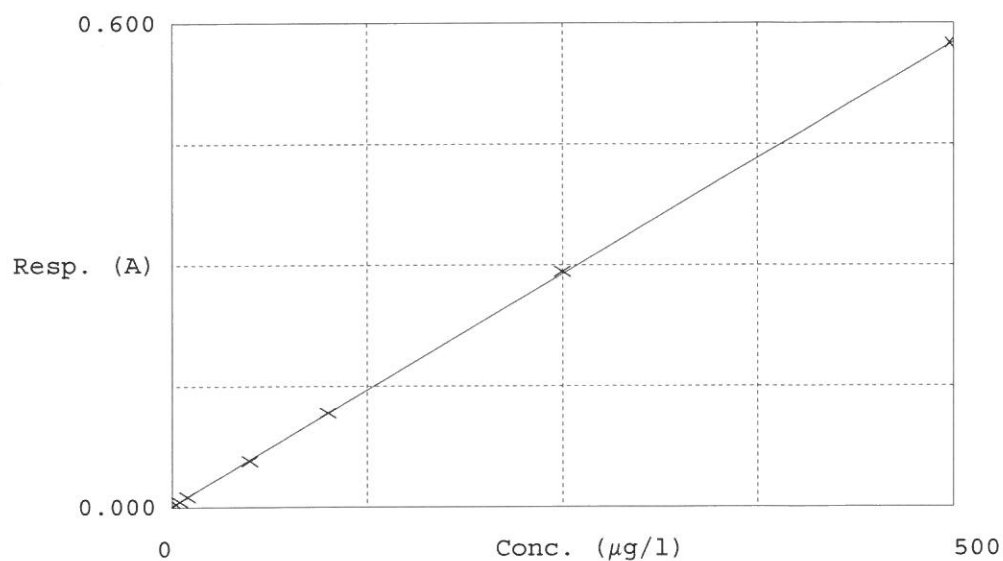

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.0408	0.0000	
2	5.0PPBCN	0.007	4.6531	5.0000	
3	10PPBCN	0.013	9.9584	10.0000	
4	50PPBCN	0.057	48.5374	50.0000	
5	100PPBCN	0.117	100.5264	100.0000	
6	250PPBCN	0.292	252.4772	250.0000	
7	500PPBCN	0.575	498.8067	500.0000	

AR

Aquakem v. 7.2AQ1

Results from time period:

Wed Dec 18 15:57:56 2019

Wed Dec 18 16:32:44 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	Cl P	0.0408	µg/l	12/18/2019 15:57:56	
5.OPPBCN	A	Reactive	Cl P	4.6531	µg/l	12/18/2019 15:57:57	
10PPBCN	A	Reactive	Cl P	9.9584	µg/l	12/18/2019 15:57:58	
50PPBCN	A	Reactive	Cl P	48.5374	µg/l	12/18/2019 15:57:59	
100PPBCN	A	Reactive	Cl P	100.5264	µg/l	12/18/2019 15:58:00	
250PPBCN	A	Reactive	Cl P	252.4772	µg/l	12/18/2019 15:58:01	
500PPBCN	A	Reactive	Cl P	498.8067	µg/l	12/18/2019 15:58:02	
ICV1	S	Reactive	Cl P	95.6461	µg/l	12/18/2019 16:29:20	
ICB1	S	Reactive	Cl P	0.4122	µg/l	12/18/2019 16:29:21	
CCV1	S	Reactive	Cl P	239.0886	µg/l	12/18/2019 16:29:22	
CCB1	S	Reactive	Cl P	0.1939	µg/l	12/18/2019 16:29:23	
PB125588BL	S	Reactive	Cl P	0.103	µg/l	12/18/2019 16:29:24	
K6310-04	S	Reactive	Cl P	-0.0531	µg/l	12/18/2019 16:29:25	
K6359-03	S	Reactive	Cl P	-0.2202	µg/l	12/18/2019 16:29:26	
K6359-03DUP	S	Reactive	Cl P	0.0579	µg/l	12/18/2019 16:29:27	
K6359-04	S	Reactive	Cl P	-0.2121	µg/l	12/18/2019 16:29:28	
K6359-05	S	Reactive	Cl P	0.1923	µg/l	12/18/2019 16:29:29	
K6360-02	S	Reactive	Cl P	0.0958	µg/l	12/18/2019 16:29:30	
CCV2	S	Reactive	Cl P	259.6892	µg/l	12/18/2019 16:32:43	
CCB2	S	Reactive	Cl P	0.1497	µg/l	12/18/2019 16:32:44	