

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AP

Instrument ID : Konelab

12/20/2019 10:27

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.982	0.0	0.106	
ICB1	-0.004	0.0	0.008	
CCV1	0.982	0.0	0.106	
CCB1	-0.001	0.0	0.008	
PB125592BL	-0.000	0.0	0.008	
PB125592BS	0.998	0.0	0.108	
K6348-01	-0.000	0.0	0.008	
K6348-01DUP	0.002	0.0	0.008	
K6348-01MS	0.924	0.0	0.101	
K6348-01MSD	0.923	0.0	0.101	
CCV2	0.974	0.0	0.106	
CCB2	-0.004	0.0	0.008	

N	12
Mean	0.481
SD	0.5045
CV%	104.81

Aquakem v. 7.2AQ1

Results from time period:

Fri Dec 20 09:46:14 2019

Fri Dec 20 10:19:03 2019

AG

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0532	mg/l	12/20/2019 9:46:14	
0.1PPM	A	Phenolics-	P	0.1048	mg/l	12/20/2019 9:46:15	
0.25PPM	A	Phenolics-	P	0.2562	mg/l	12/20/2019 9:46:16	
0.50PPM	A	Phenolics-	P	0.4867	mg/l	12/20/2019 9:46:17	
1.0PPM	A	Phenolics-	P	0.9939	mg/l	12/20/2019 9:46:18	
2.0PPM	A	Phenolics-	P	2.0053	mg/l	12/20/2019 9:46:19	
ICV1	S	Phenolics-	P	0.9819	mg/l	12/20/2019 10:15:04	
ICB1	S	Phenolics-	P	-0.004	mg/l	12/20/2019 10:15:05	
CCV1	S	Phenolics-	P	0.9824	mg/l	12/20/2019 10:15:06	
CCB1	S	Phenolics-	P	-0.0011	mg/l	12/20/2019 10:15:07	
PB125592BL	S	Phenolics-	P	-0.0002	mg/l	12/20/2019 10:15:08	
PB125592BS	S	Phenolics-	P	0.9979	mg/l	12/20/2019 10:15:09	
K6348-01	S	Phenolics-	P	-0.0002	mg/l	12/20/2019 10:15:10	
K6348-01DUP	S	Phenolics-	P	0.0017	mg/l	12/20/2019 10:15:11	
K6348-01MS	S	Phenolics-	P	0.9244	mg/l	12/20/2019 10:15:12	
K6348-01MSD	S	Phenolics-	P	0.923	mg/l	12/20/2019 10:15:13	
CCV2	S	Phenolics-	P	0.974	mg/l	12/20/2019 10:15:14	
CCB2	S	Phenolics-	P	-0.0036	mg/l	12/20/2019 10:15:15	

LB106873

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AD

Instrument ID : Konelab

12/20/2019 9:48


Test Phenolics-

Accepted 12/20/2019 9:48

Factor 10
Bias 0.008

Coeff. of det. 0.999887

Errors

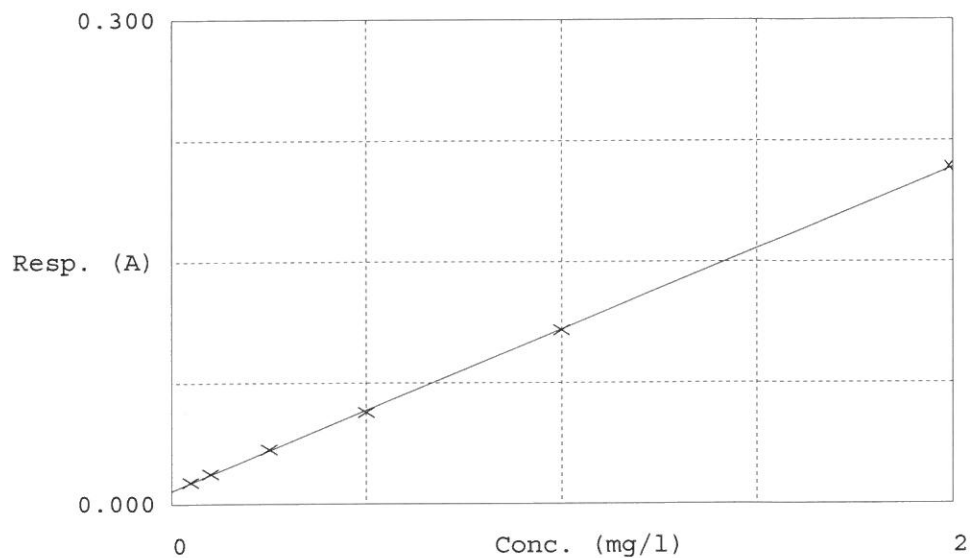

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.014	0.0532	0.0500	
2	Phenol-2	0.019	0.1048	0.1000	
3	Phenol-2	0.034	0.2562	0.2500	
4	Phenol-2	0.057	0.4867	0.5000	
5	Phenol-2	0.108	0.9939	1.0000	
6	Phenol-2	0.209	2.0053	2.0000	