

LB106874

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : no

Instrument ID : Konelab

12/20/2019 12:32

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.576	0.0	0.110	
ICB1	0.808	0.0	0.002	
CCV1	238.868	0.0	0.277	
CCB1	0.594	0.0	0.002	
PB125614BL	0.686	0.0	0.002	
PB125614BS	95.869	0.0	0.112	
MIDPB125614	242.184	0.0	0.281	
K6348-01	1.103	0.0	0.003	
K6348-01DUP	1.061	0.0	0.002	
K6348-01MS	38.897	0.0	0.046	
K6348-01MSD	31.610	0.0	0.038	
CCV2	260.514	0.0	0.302	
CCB2	0.655	0.0	0.002	

N	13
Mean	77.494
SD	102.5348
CV%	132.31

AC

Aquakem v. 7.2AQ1

Results from time period:

Fri Dec 20 11:16:59 2019

Fri Dec 20 12:11:52 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.4224	µg/l	12/20/2019 11:16:59	
5.OPPBCN	A	Total CN	P	5.3867	µg/l	12/20/2019 11:17:00	
10PPBCN	A	Total CN	P	10.0821	µg/l	12/20/2019 11:17:01	
50PPBCN	A	Total CN	P	49.1459	µg/l	12/20/2019 11:17:02	
100PPBCN	A	Total CN	P	99.3198	µg/l	12/20/2019 11:17:03	
250PPBCN	A	Total CN	P	250.8544	µg/l	12/20/2019 11:17:04	
500PPBCN	A	Total CN	P	499.7887	µg/l	12/20/2019 11:17:05	
ICV1	S	Total CN	P	94.576	µg/l	12/20/2019 11:42:12	
ICB1	S	Total CN	P	0.8083	µg/l	12/20/2019 11:42:13	
CCV1	S	Total CN	P	238.8676	µg/l	12/20/2019 11:42:14	
CCB1	S	Total CN	P	0.5941	µg/l	12/20/2019 11:42:15	
PB125614BL	S	Total CN	P	0.686	µg/l	12/20/2019 11:42:16	
PB125614BS	S	Total CN	P	95.8689	µg/l	12/20/2019 11:42:17	
MIDPB125614	S	Total CN	P	242.1841	µg/l	12/20/2019 11:42:18	
K6348-01	S	Total CN	P	1.1032	µg/l	12/20/2019 11:42:19	
K6348-01DUP	S	Total CN	P	1.061	µg/l	12/20/2019 11:42:20	
K6348-01MS	S	Total CN	P	38.8968	µg/l	12/20/2019 11:42:21	
K6348-01MSD	S	Total CN	P	31.6103	µg/l	12/20/2019 12:11:50	
CCV2	S	Total CN	P	260.514	µg/l	12/20/2019 12:11:51	
CCB2	S	Total CN	P	0.6551	µg/l	12/20/2019 12:11:52	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DR

Instrument ID : Konelab

12/20/2019 11:18


Test Total CN

Accepted 12/20/2019 11:18

Factor 867.1
Bias 0.001

Coeff. of det. 0.999989

Errors

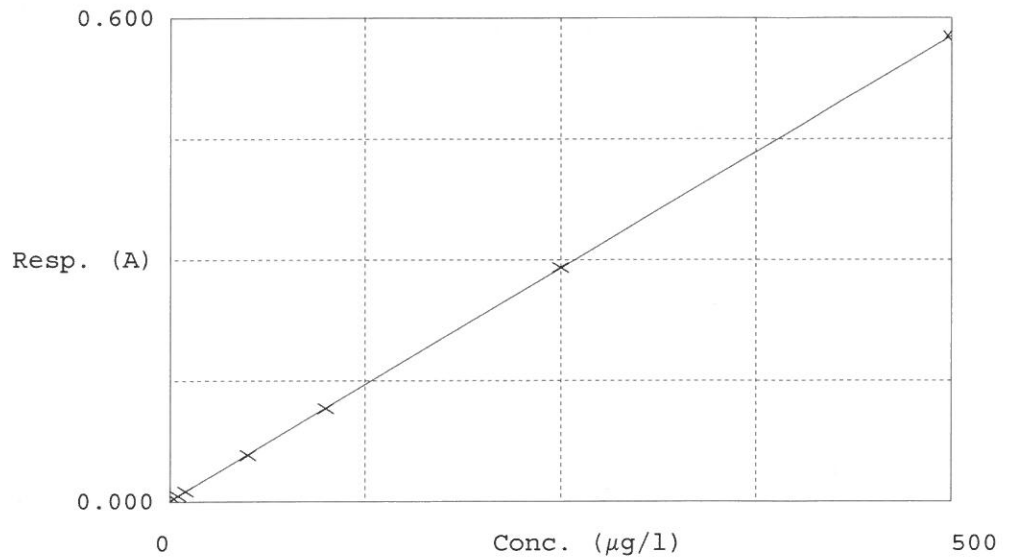

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.4224	0.0000	
2	5.0PPBCN	0.007	5.3867	5.0000	
3	10PPBCN	0.013	10.0821	10.0000	
4	50PPBCN	0.058	49.1459	50.0000	
5	100PPBCN	0.116	99.3198	100.0000	
6	250PPBCN	0.291	250.8544	250.0000	
7	500PPBCN	0.578	499.7887	500.0000	