

IC-2 9056/notes

MDL for all analyses

AK 12-28-19

Clear table

ident	concentra tion F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-19_	12/19/19 15:26		CT/AP
STD2	0.2500	0.3990	0.3800	1.2380	0.3170	0.3550	2.0020	2019-12-19_	12/19/19 15:56		CT/AP
STD3	0.4400	0.6420	0.6580	2.2270	0.5560	0.9870	3.3430	2019-12-19_	12/19/19 16:25		CT/AP
STD4	0.8110	1.1640	1.1660	3.8820	0.9740	2.0690	5.8260	2019-12-19_	12/19/19 16:54		CT/AP
STD5	1.9030	2.8750	2.8740	9.5760	2.3840	5.1810	14.2170	2019-12-19_	12/19/19 17:23		CT/AP
STD6	3.8700	5.8950	5.9010	19.6930	4.9110	9.9480	29.3600	2019-12-19_	12/19/19 17:52		CT/AP
STD7	5.1270	7.6250	7.6200	25.3850	6.3580	12.4600	38.2530	2019-12-19_	12/19/19 18:21		CT/AP
ICV	2.0360	2.9970	2.9950	9.9910	2.4820	5.3130	14.8340	2019-12-19_	12/19/19 19:49		CT/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-19_	12/19/19 20:18		CT/AP
CCV	1.9080	2.9990	2.8540	9.6900	2.4830	4.9510	14.0390	2019-12-23_	12/23/19 10:43		CT/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-23_	12/23/19 11:15		CT/AP
LB106931BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-23_	12/23/19 11:45		CT/AP
LB106931BSW	1.8760	2.9870	2.8770	9.6300	2.4910	5.0390	13.9780	2019-12-23_	12/23/19 12:14		CT/AP
K5111-09	0.1930	0.2430	0.2540	0.8280	0.2260	0.0810	1.3600	2019-12-23_	12/23/19 13:54		CT/AP
K5111-09RE	0.2510	0.4010	0.3860	1.2540	0.3410	0.3470	2.0180	2019-12-23_	12/23/19 14:23		CT/AP
CCV	1.9290	3.0000	2.8810	9.6550	2.5300	5.4030	13.9160	2019-12-23_	12/23/19 14:53		CT/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2019-12-23_	12/23/19 15:22		CT/AP


CALIBRATION OF COMPONENT F-

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.0755513 \cdot A + 1.93672$
 RSD: 5.227 %
 Correlation coefficient: 0.998845

IC2 CAL

12-19-19

AL

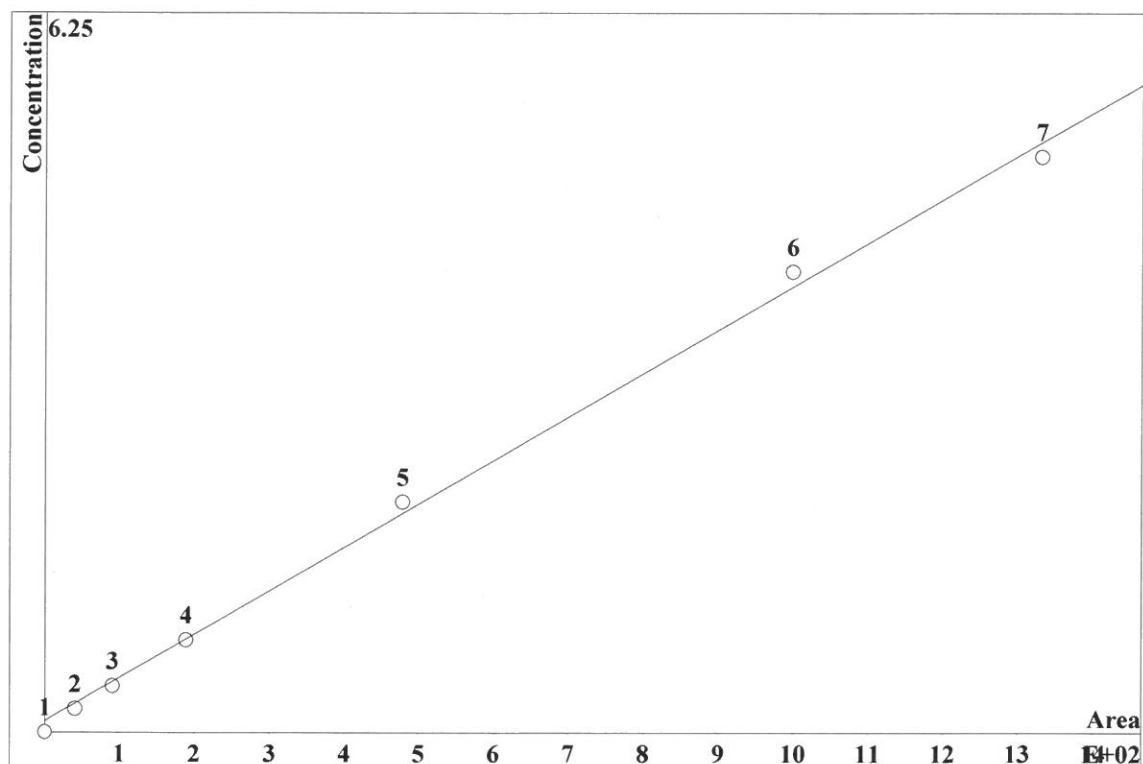

K3 = 0 K2 = 0 K1 = 0.0755513 K0 = 1.93672

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	1.602	40.47	0.2	20	5.516		
3	3.353	90.84	0.4	20	5.516		
4	7.546	189	0.8	20	5.516		
5	20.92	478.2	2	20	5.516		
6	45.31	998.7	4	20	5.516		
7	62.11	1332	5	20	5.516		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.140776 \cdot A + 1.87523$
 RSD: 3.786 %
 Correlation coefficient: 0.999394

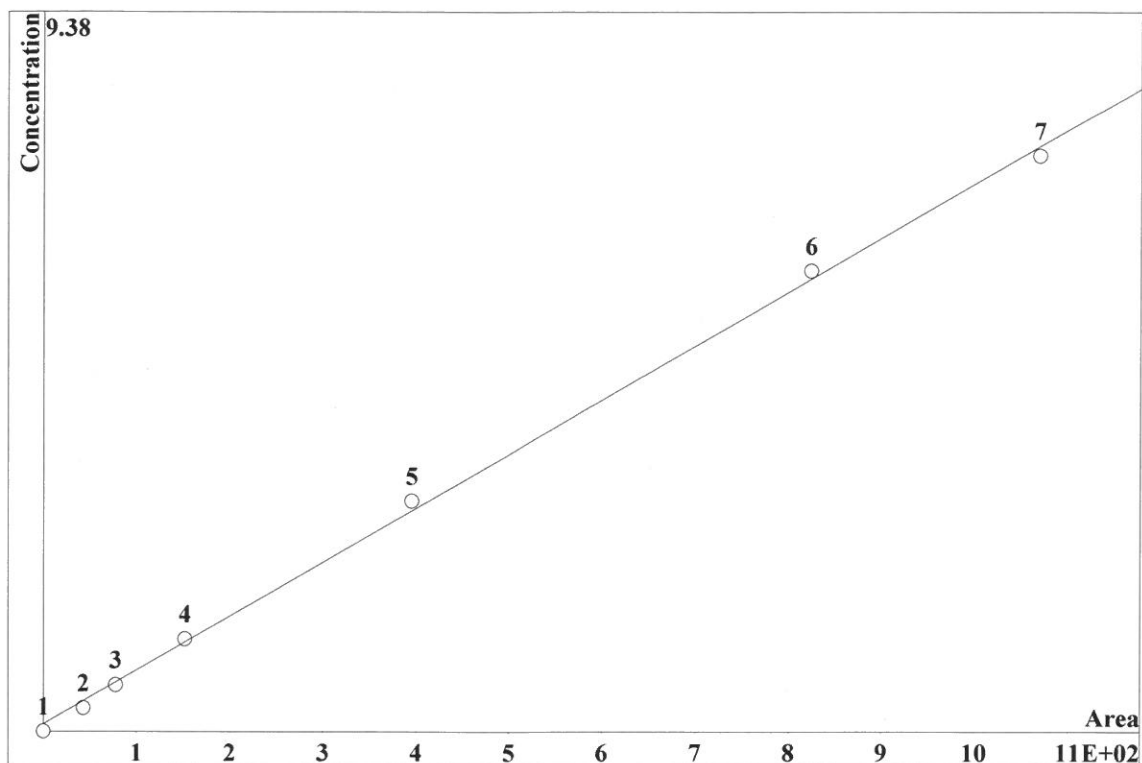

K3 = 0 K2 = 0 K1 = 0.140776 K0 = 1.87523

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.573	43.41	0.3	20	8.443		
3	5.183	77.84	0.6	20	8.443		
4	10.01	152	1.2	20	8.443		
5	26.33	395.2	3	20	8.443		
6	55.7	824.2	6	20	8.443		
7	72.45	1070	7.5	20	8.443		

ŷ

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.0627248 \cdot A + 2.30587$
 RSD: 3.646 %
 Correlation coefficient: 0.999438

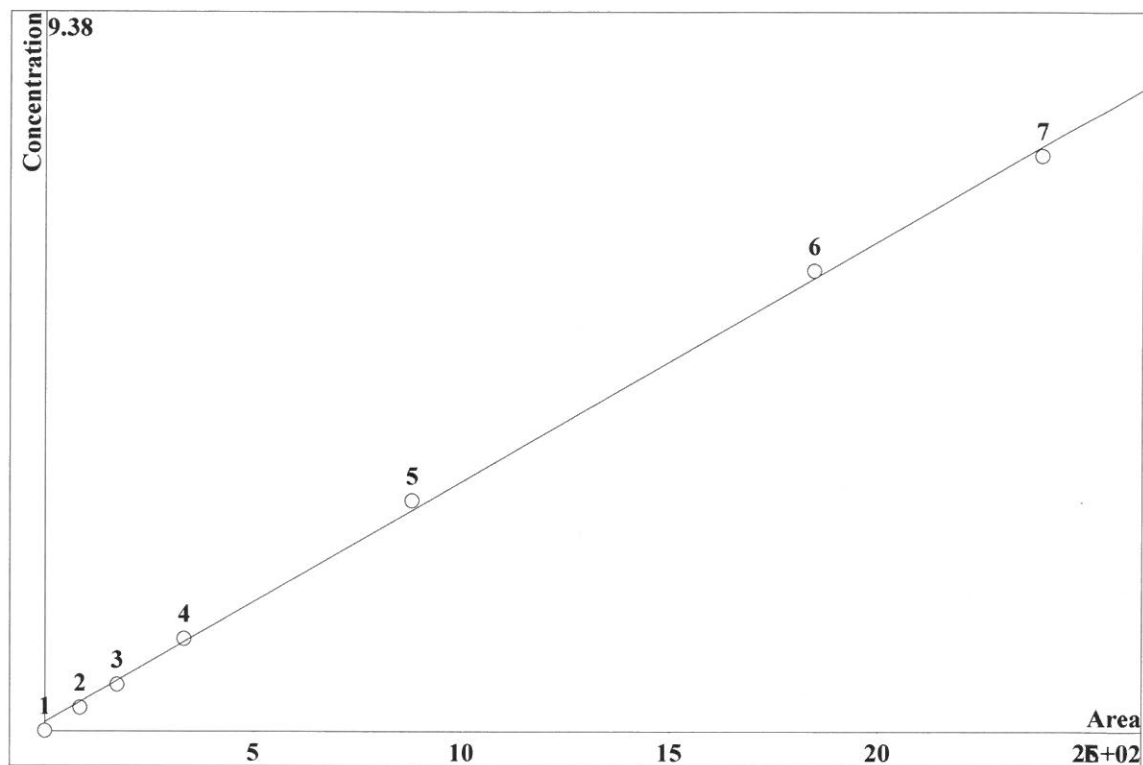

K3 = 0 K2 = 0 K1 = 0.0627248 K0 = 2.30587

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.615	84.53	0.3	20	10.18		
3	9.322	173.1	0.6	20	10.18		
4	17.96	334.9	1.2	20	10.18		
5	46.4	879.7	3	20	10.18		
6	93.12	1845	6	20	10.18		
7	120	2393	7.5	20	10.18		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.316728 \cdot A + 7.75699$
 RSD: 3.568 %
 Correlation coefficient: 0.999462

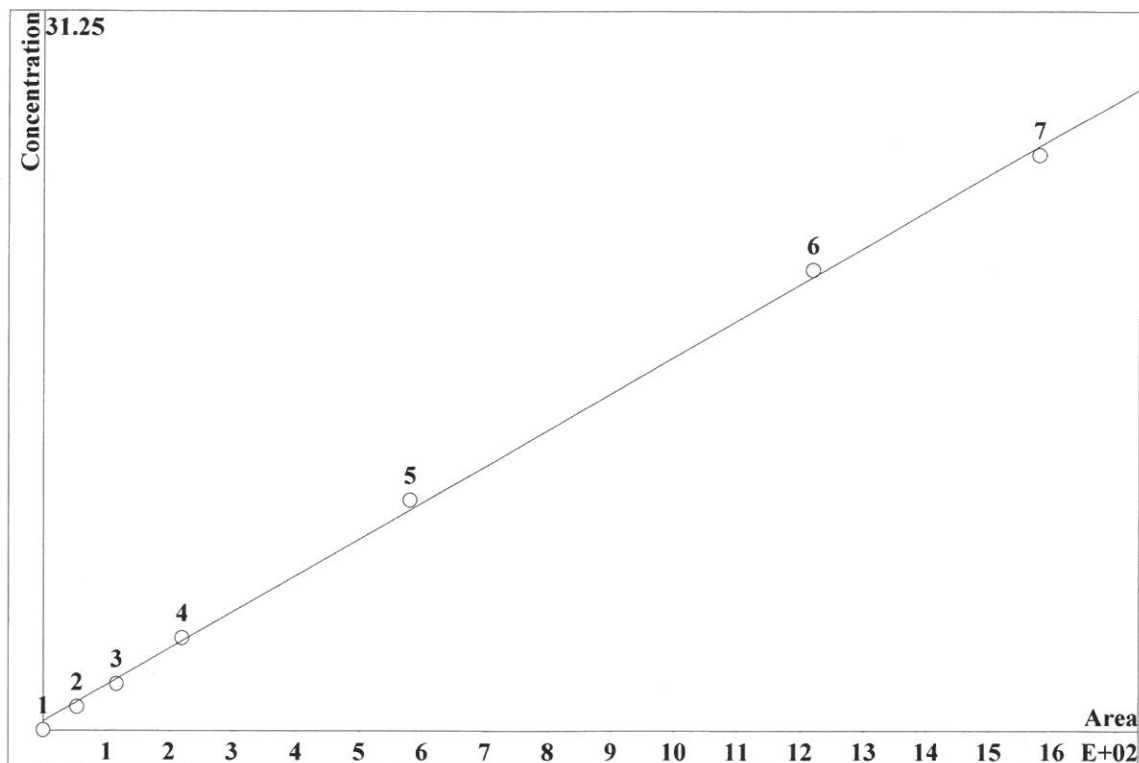

K3 = 0 K2 = 0 K1 = 0.316728 K0 = 7.75699

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.506	53.65	1	20	13.07		
3	5.233	116.1	2	20	13.07		
4	10.12	220.6	4	20	13.07		
5	26.95	580.2	10	20	13.07		
6	57.56	1219	20	20	13.07		
7	75.01	1578	25	20	13.07		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.0567155 \cdot A + 1.9162$
 RSD: 3.923 %
 Correlation coefficient: 0.999349

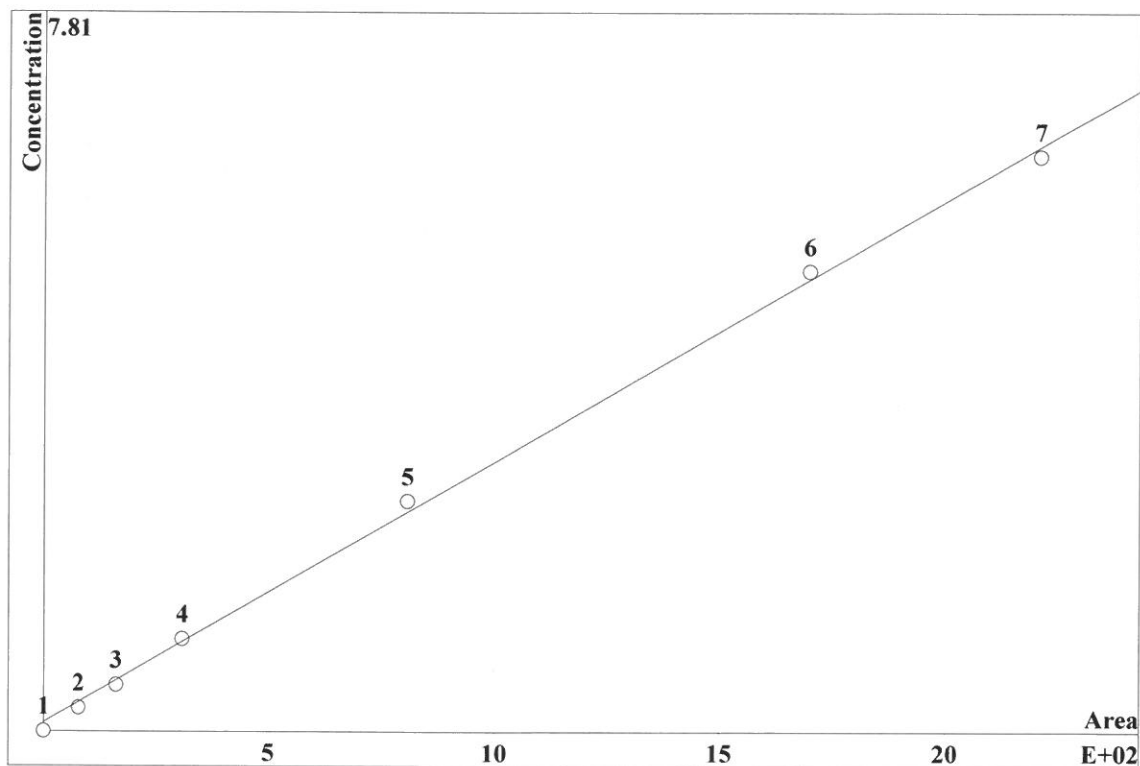

K3 = 0 K2 = 0 K1 = 0.0567155 K0 = 1.9162

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.046	77.91	0.25	20	15.04		
3	6.249	162.2	0.5	20	15.04		
4	11.98	309.8	1	20	15.04		
5	31.2	806.9	2.5	20	15.04		
6	65.71	1698	5	20	15.04		
7	85.55	2208	6.25	20	15.04		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.0942908 \cdot A - 3.46159$
 RSD: 2.433 %
 Correlation coefficient: 0.999750

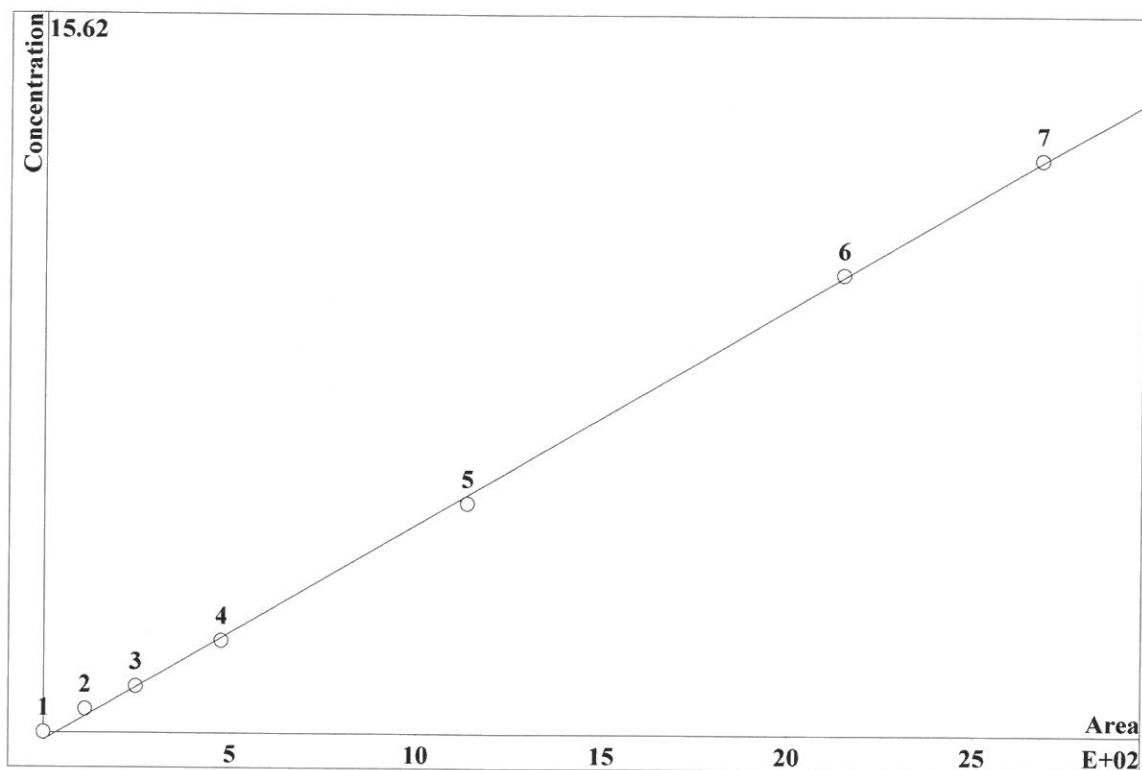

K3 = 0 K2 = 0 K1 = 0.0942908 K0 = -3.46159

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.415	112	0.5	20	20.37		
3	5.344	246	1	20	20.37		
4	10.51	475.5	2	20	20.37		
5	26.2	1136	5	20	20.37		
6	51.59	2147	10	20	20.37		
7	65.47	2680	12.5	20	20.37		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-121919.mtw
 Equation: $Q = 0.181366 \cdot A + 12.4427$
 RSD: 4.550 %
 Correlation coefficient: 0.999125

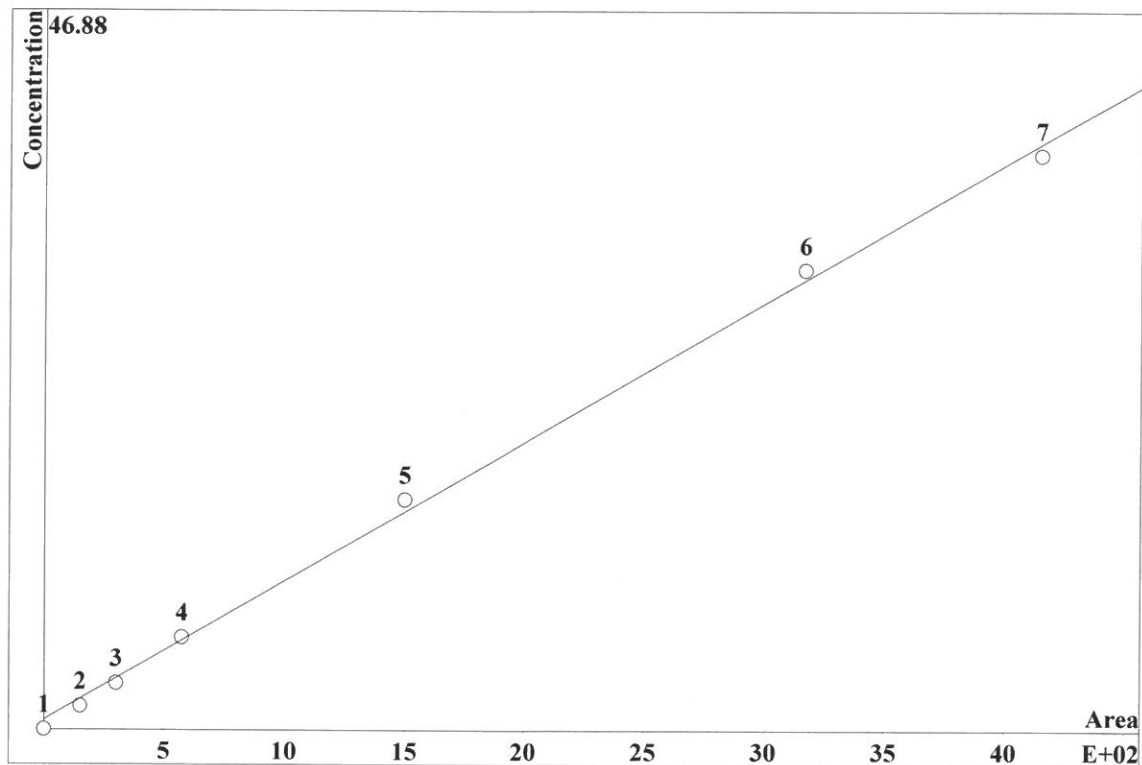

K3 = 0 K2 = 0 K1 = 0.181366 K0 = 12.4427

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.868	152.1	1.5	20	23.43		
3	7.718	300.1	3	20	23.43		
4	14.7	573.8	6	20	23.43		
5	38.7	1499	15	20	23.43		
6	82.78	3169	30	20	23.43		
7	108.7	4150	37.5	20	23.43		

Report date: 12/23/2019 11:14:07 AM
Printed by: wet


Ident: STD1
Analysis from: 12/19/2019 3:26:59 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:00 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24042

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

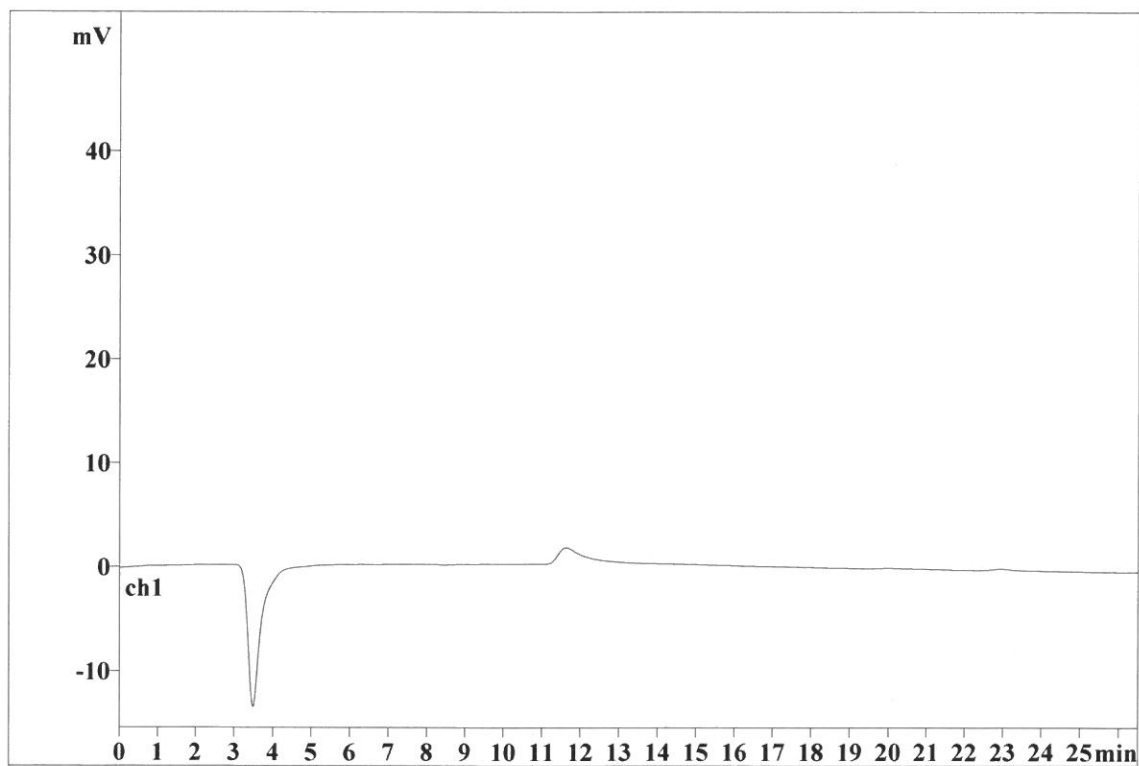

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:14:24 AM
Printed by: wet


Ident: STD2
Analysis from: 12/19/2019 3:56:07 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:00 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24043

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

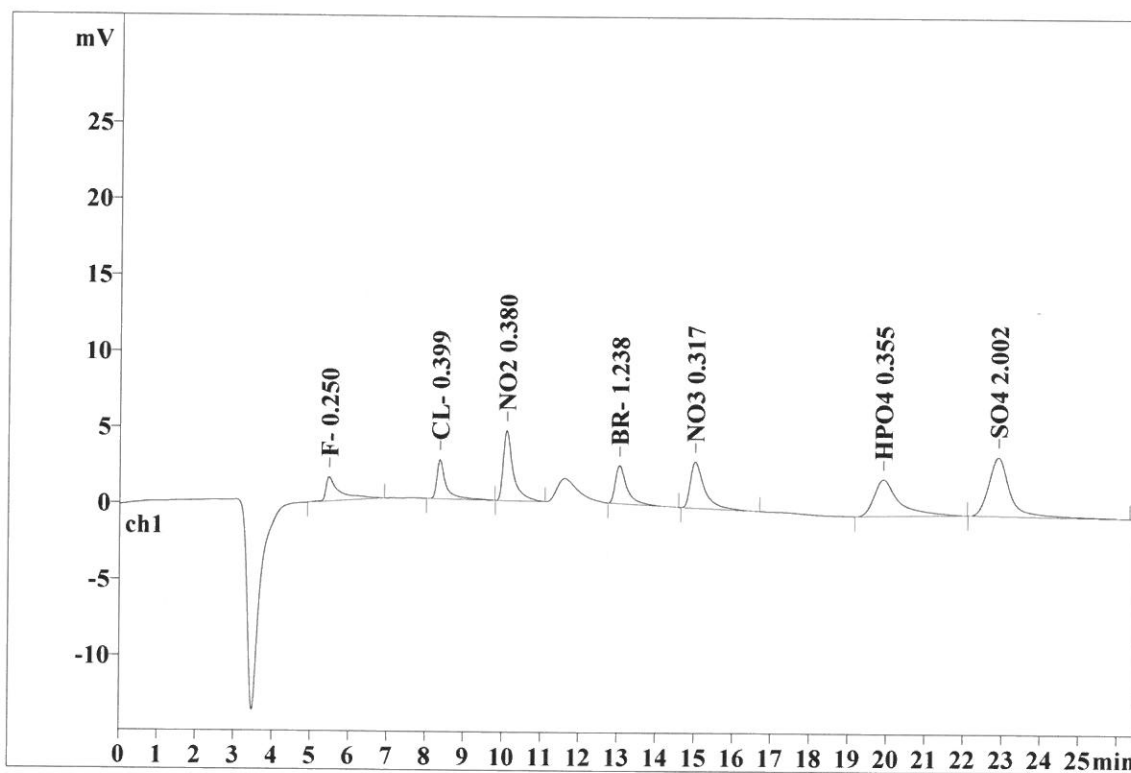

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.46	0.274	1.60	7.76	40.468	7.17
2	8.35	0.206	2.57	12.46	43.408	7.69
3	10.08	0.245	4.61	22.37	84.529	14.98
4	13.03	0.294	2.51	12.15	53.654	9.51
5	15.00	0.350	3.04	14.76	77.906	13.81
6	19.89	0.594	2.41	11.70	112.029	19.86
7	22.87	0.536	3.87	18.75	152.123	26.97
7	26.50	0.357	20.62	99.96	564.118	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:14:38 AM
Printed by: wet


Ident: STD3
Analysis from: 12/19/2019 4:25:15 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:01 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24044

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

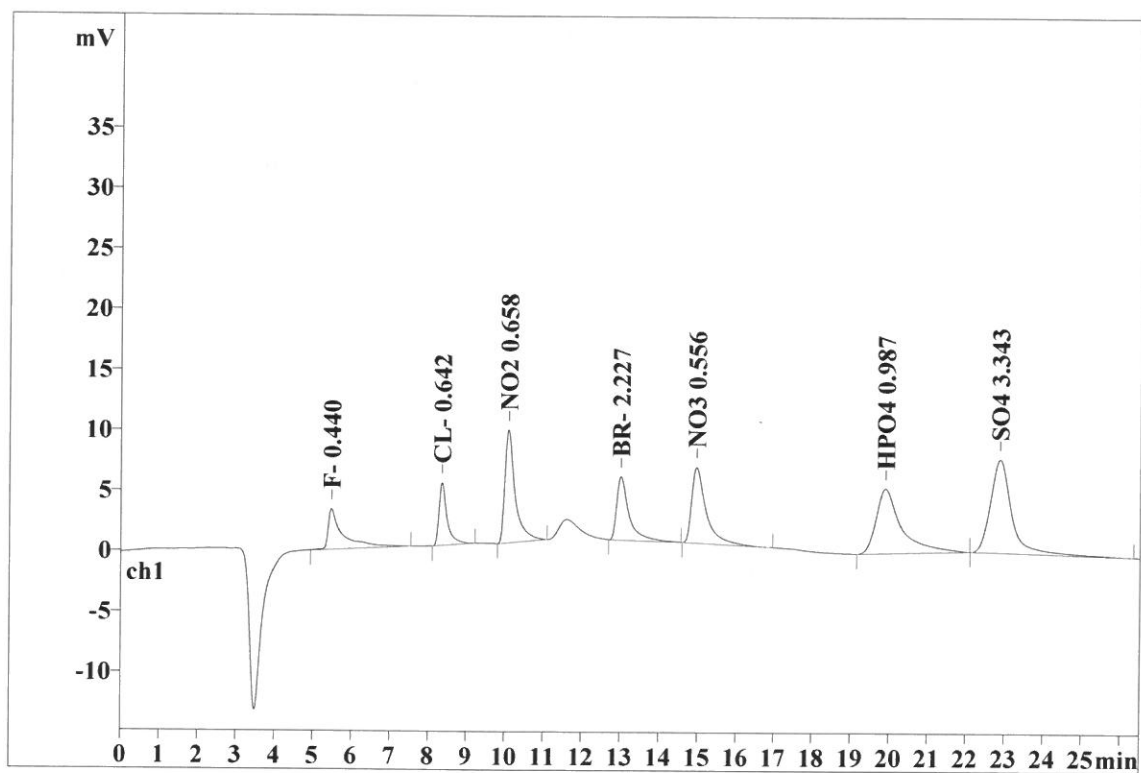

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.46	0.273	3.35	7.90	90.838	7.79
2	8.34	0.204	5.18	12.22	77.838	6.67
3	10.08	0.250	9.32	21.98	173.143	14.85
4	13.00	0.295	5.23	12.34	116.126	9.96
5	14.96	0.350	6.25	14.74	162.230	13.91
6	19.90	0.588	5.34	12.60	246.023	21.09
7	22.88	0.533	7.72	18.20	300.076	25.73
7	26.50	0.356	42.40	99.99	1166.274	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:14:51 AM
Printed by: wet


Ident: STD4
Analysis from: 12/19/2019 4:54:22 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:01 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24045

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

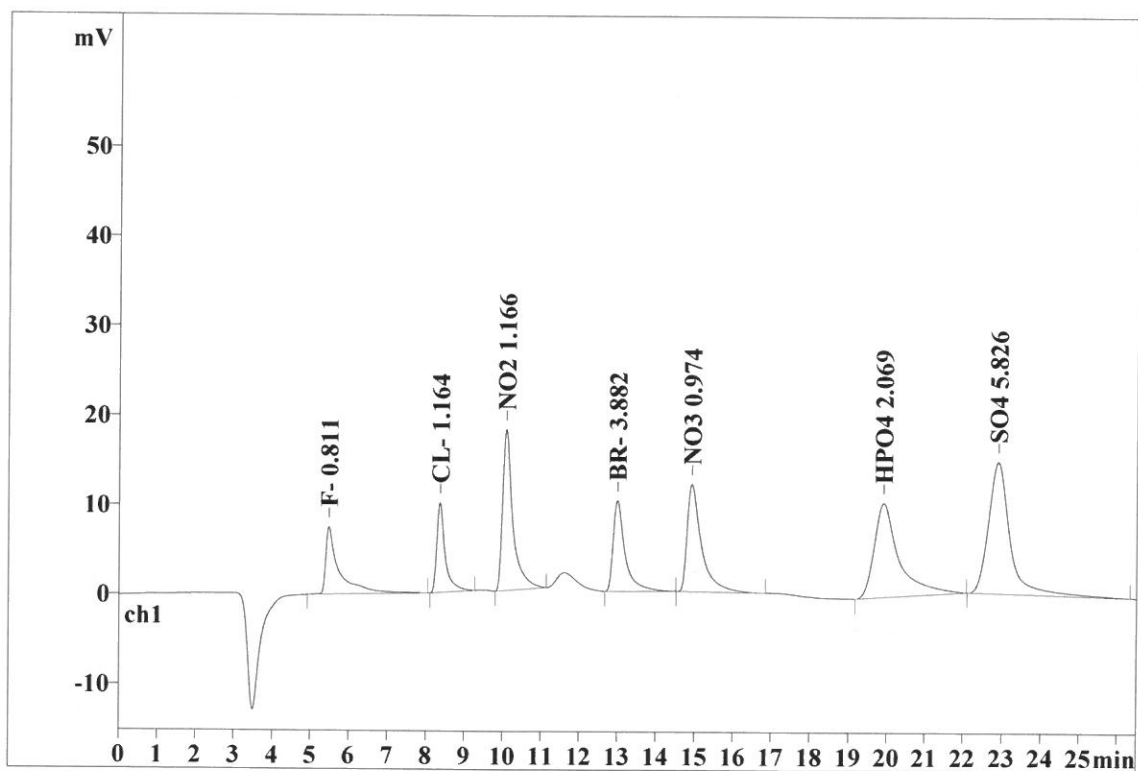

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.47	0.258	7.54	9.11	188.985	8.38
2	8.35	0.204	10.01	12.09	151.994	6.74
3	10.07	0.248	17.96	21.68	334.935	14.85
4	12.98	0.292	10.12	12.22	220.644	9.78
5	14.91	0.350	11.98	14.46	309.778	13.73
6	19.90	0.579	10.50	12.68	475.545	21.08
7	22.89	0.531	14.70	17.75	573.814	25.44
7	26.50	0.352	82.82	99.99	2255.695	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:15:01 AM
Printed by: wet


Ident: STD5
Analysis from: 12/19/2019 5:23:31 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:01 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24046

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

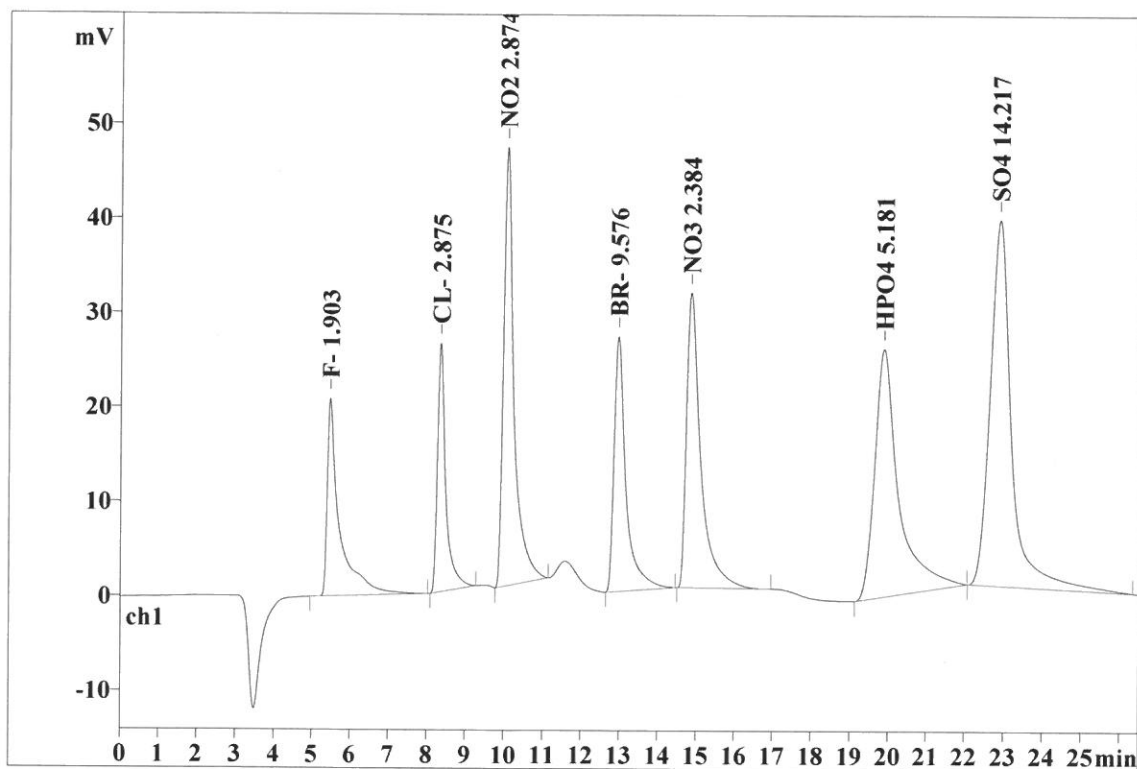

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.47	0.243	20.92	9.65	478.173	8.28
2	8.34	0.200	26.32	12.15	395.195	6.84
3	10.04	0.253	46.40	21.41	879.705	15.23
4	12.95	0.286	26.95	12.44	580.168	10.05
5	14.84	0.350	31.19	14.40	806.924	13.97
6	19.87	0.555	26.20	12.09	1135.752	19.67
7	22.87	0.524	38.70	17.86	1499.142	25.96
7	26.50	0.345	216.68	100.00	5775.059	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:15:11 AM
Printed by: wet


Ident: STD6
Analysis from: 12/19/2019 5:52:39 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:01 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24047

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

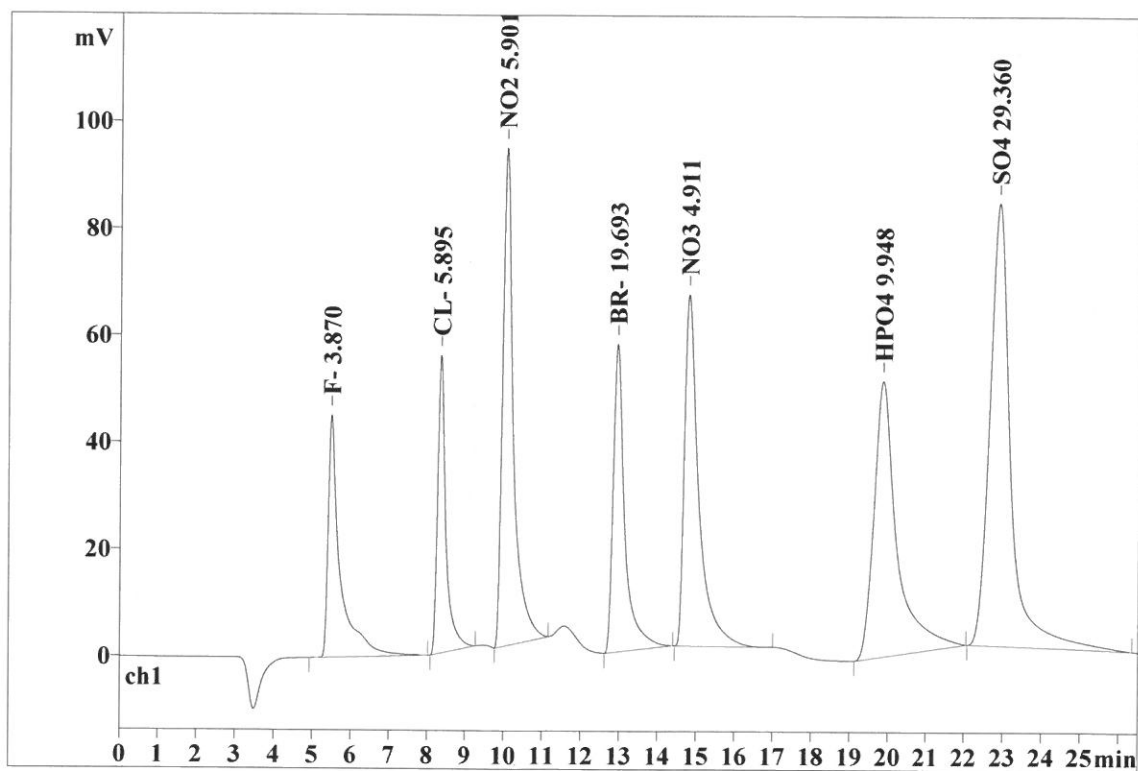

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.48	0.240	45.31	10.03	998.717	8.39
2	8.34	0.198	55.70	12.33	824.179	6.93
3	10.03	0.269	93.12	20.61	1844.817	15.50
4	12.93	0.281	57.56	12.74	1219.057	10.24
5	14.79	0.350	65.71	14.55	1698.186	14.27
6	19.85	0.535	51.59	11.42	2146.735	18.04
7	22.87	0.515	82.77	18.32	3169.042	26.63
7	26.50	0.341	451.76	100.00	11900.734	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:15:25 AM
Printed by: wet


Ident: STD7
Analysis from: 12/19/2019 6:21:47 PM
File: _2019-12-19_

Last save: 12/20/2019 9:09:59 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24048

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

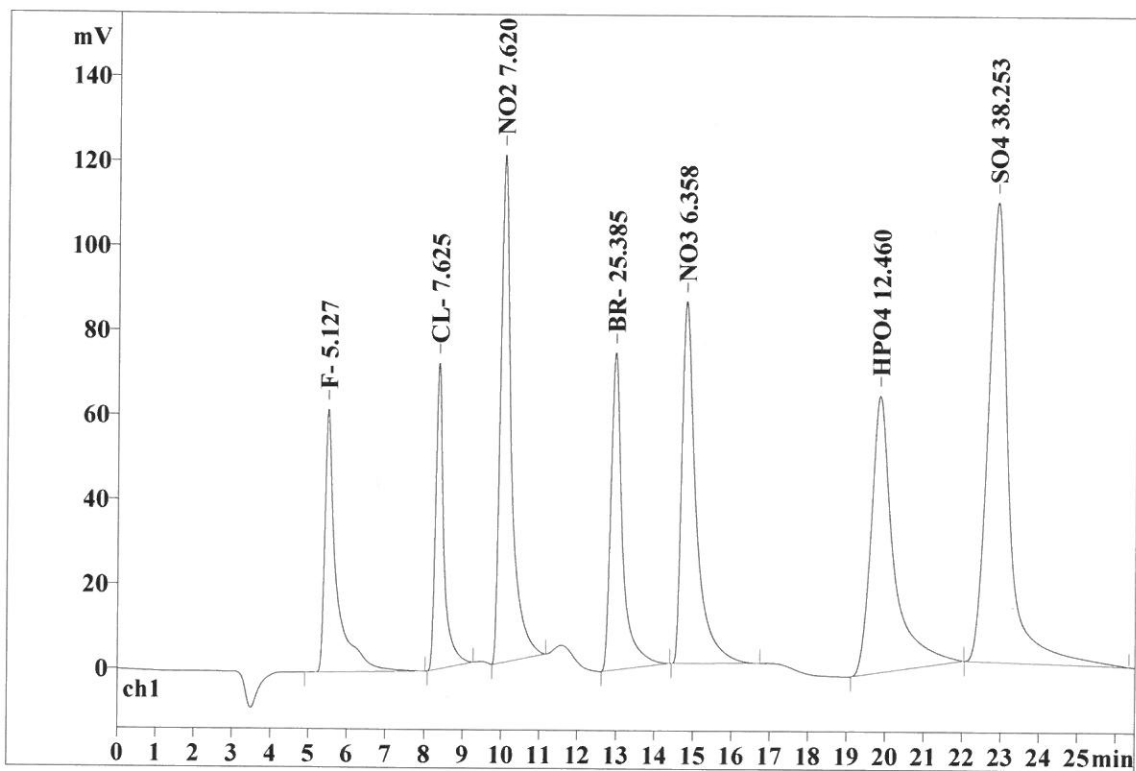

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.49	0.240	62.11	10.54	1331.550	8.64
2	8.34	0.198	72.44	12.29	1069.966	6.94
3	10.02	0.270	120.03	20.37	2392.969	15.53
4	12.94	0.280	75.01	12.73	1578.430	10.24
5	14.78	0.350	85.55	14.52	2208.140	14.33
6	19.83	0.528	65.47	11.11	2679.590	17.39
7	22.86	0.513	108.66	18.44	4149.674	26.93
7	26.50	0.340	589.27	100.00	15410.320	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:16:05 AM
Printed by: wet


Ident: ICV
Analysis from: 12/19/2019 7:49:10 PM
File: _2019-12-19_

Last save: 12/20/2019 9:10:00 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24051

Last save: 12/19/2019 6:19

SAMPLE:
: CT/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

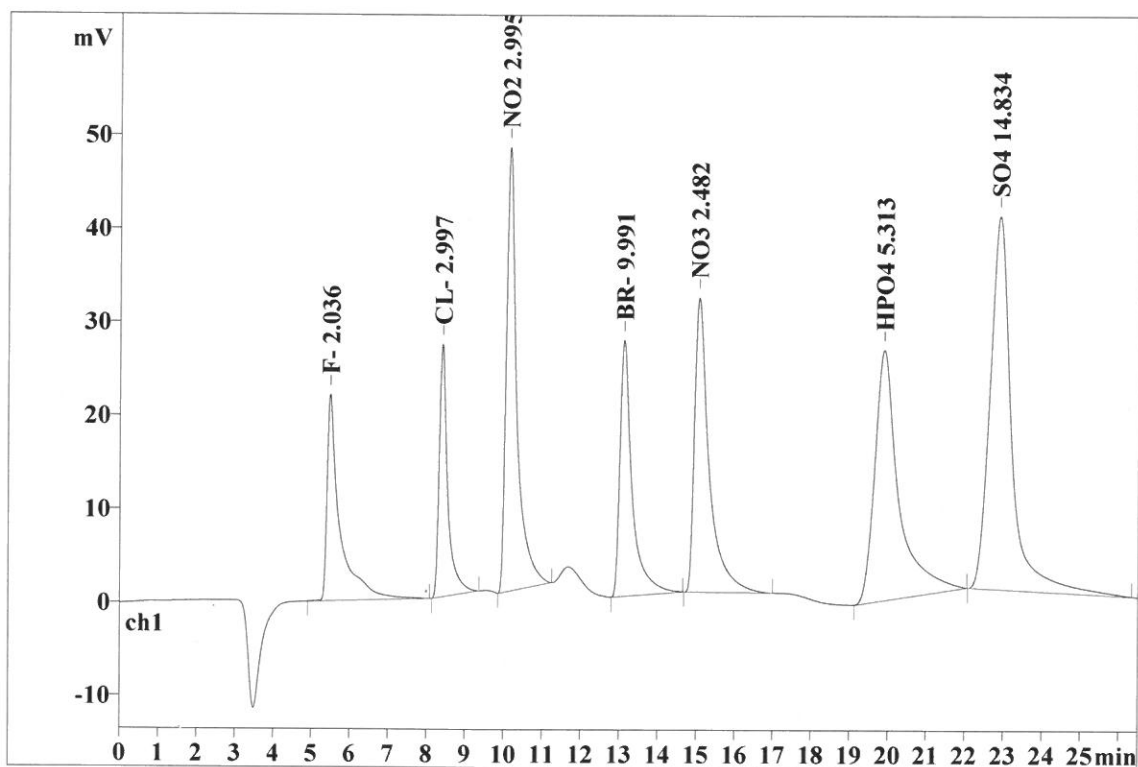

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.48	0.251	22.06	9.93	513.278	8.52
2	8.39	0.204	27.02	12.17	412.466	6.85
3	10.13	0.258	47.48	21.38	918.295	15.25
4	13.11	0.294	27.35	12.32	606.385	10.07
5	15.05	0.362	31.45	14.16	841.437	13.97
6	19.88	0.560	26.76	12.05	1163.557	19.32
7	22.88	0.531	39.94	17.99	1567.230	26.02
7	26.50	0.351	222.06	100.00	6022.648	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2019 11:16:16 AM
Printed by: wet


Ident: ICB
Analysis from: 12/19/2019 8:18:19 PM
File: _2019-12-19_

Last save: 12/20/2019 9:10:00 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24052

Last save: 12/19/2019 6:19

SAMPLE:
:
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

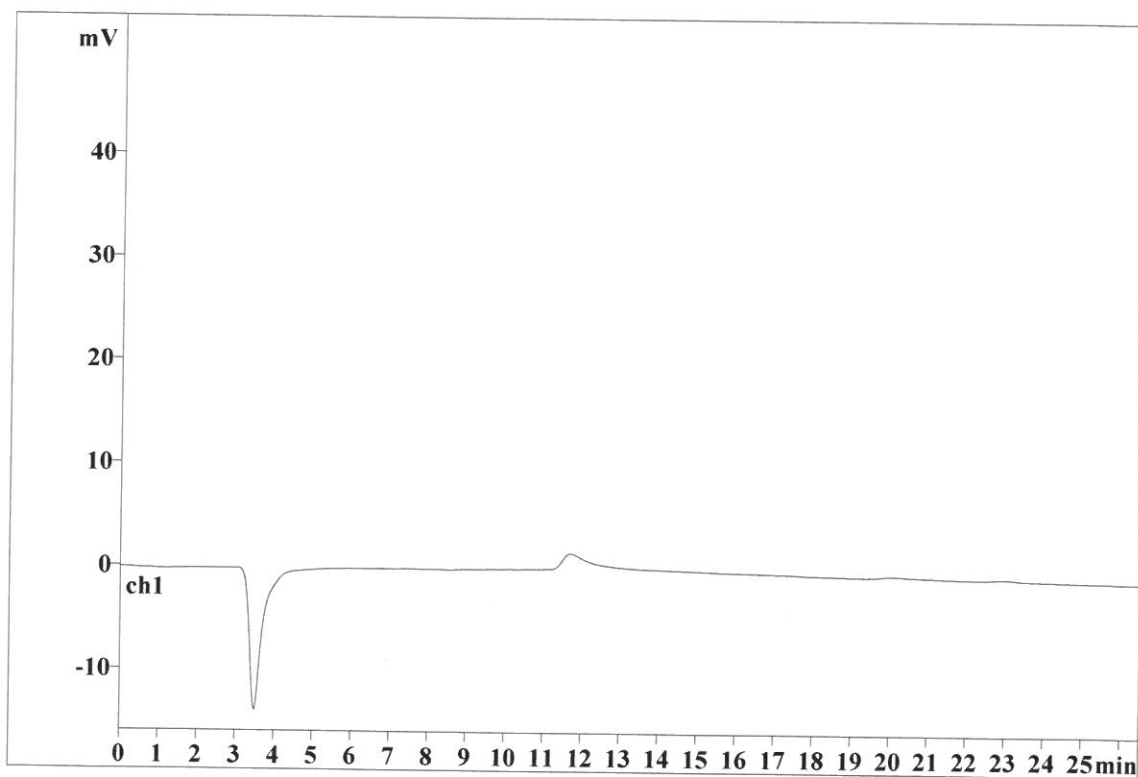

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

IC-2

9056A
water

100/mOL

Report date: 12/26/2019 11:26:42 AM
 Printed by: wet


Ident: CCV
 Analysis from: 12/23/2019 10:43:03 AM
 File: _2019-12-23_

Last save: 12/23/2019 11:09:33 AM

Method: AnionsIC2-121919.mtw
 Run operator: wet
 Analysis number: 24073

Last save: 12/20/2019 11:5

SAMPLE:
 : CT/AP
 Vial number: 2
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

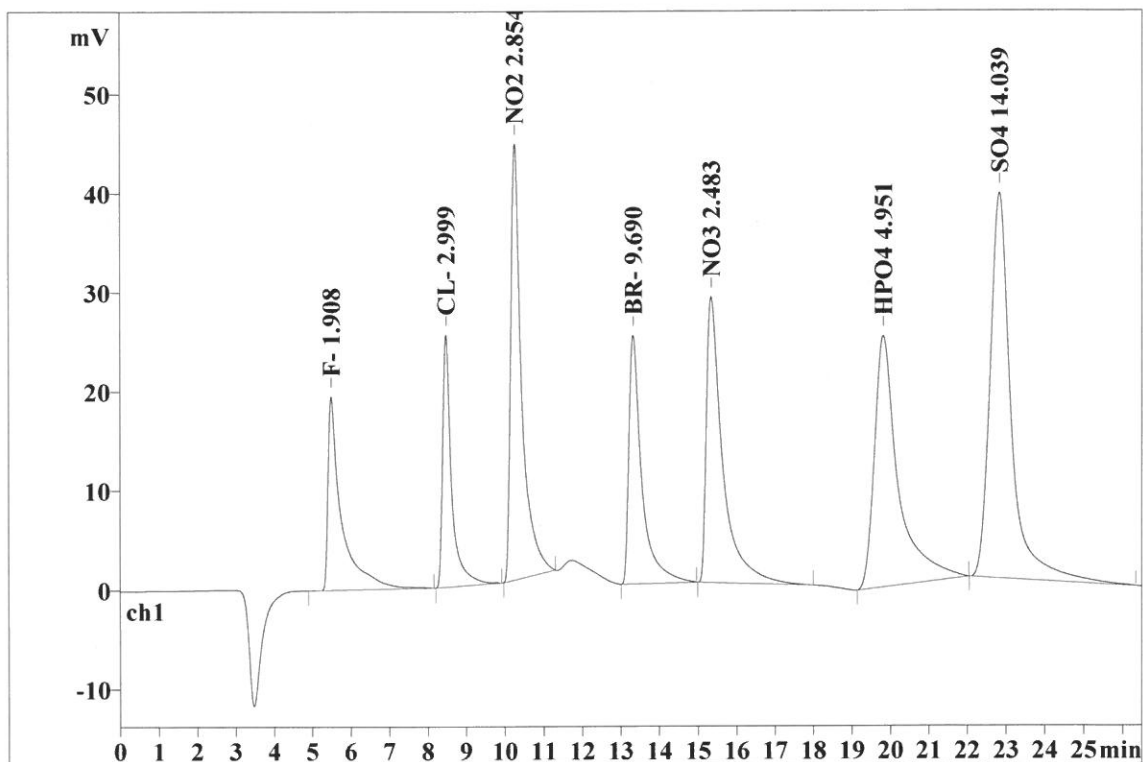

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.49	0.267	19.49	9.42	479.383	8.32
2	8.46	0.208	25.42	12.29	412.698	7.16
3	10.25	0.265	43.98	21.25	873.368	15.16
4	13.32	0.308	25.07	12.11	587.365	10.20
5	15.34	0.381	28.79	13.91	841.856	14.61
6	19.82	0.550	25.32	12.24	1086.866	18.87
7	22.84	0.521	38.86	18.78	1479.502	25.68
7	26.50	0.357	206.93	100.00	5761.037	100.00

This report has been created by IC Net
 METROHM LTD

Report date: 12/26/2019 11:26:59 AM
Printed by: wet


Ident: CCB
Analysis from: 12/23/2019 11:15:54 AM
File: _2019-12-23_

Last save: 12/23/2019 11:42:24 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24074

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

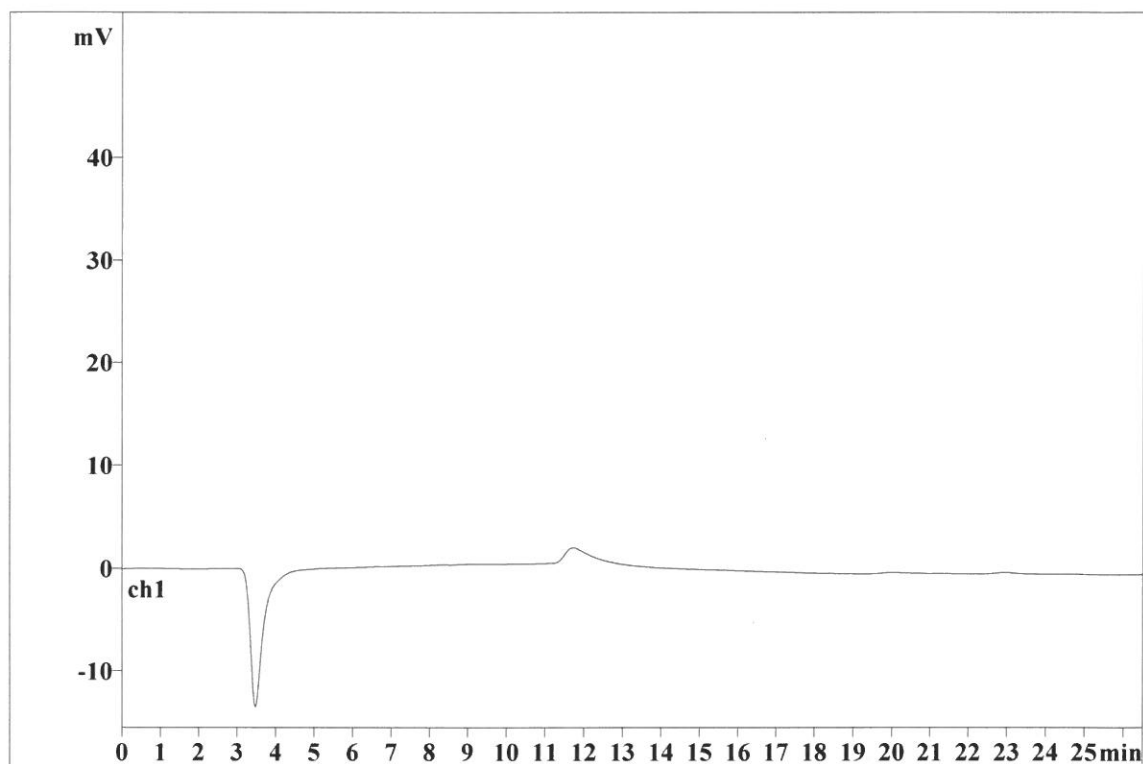

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/26/2019 11:27:08 AM
Printed by: wet


Ident: LB106931BLW
Analysis from: 12/23/2019 11:45:02 AM
File: _2019-12-23_

Last save: 12/26/2019 11:26:29 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24075

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

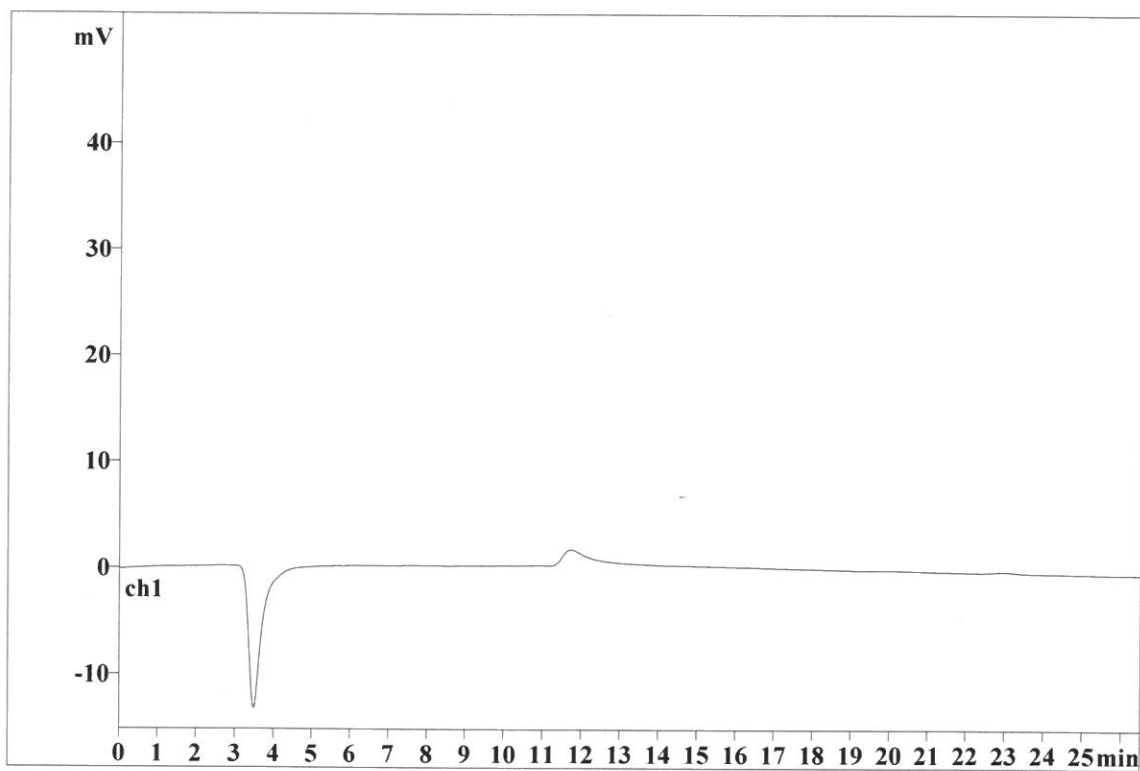

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/26/2019 11:27:20 AM
Printed by: wet


Ident: LB106931BSW
Analysis from: 12/23/2019 12:14:11 PM
File: _2019-12-23_

Last save: 12/26/2019 11:26:29 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24076

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

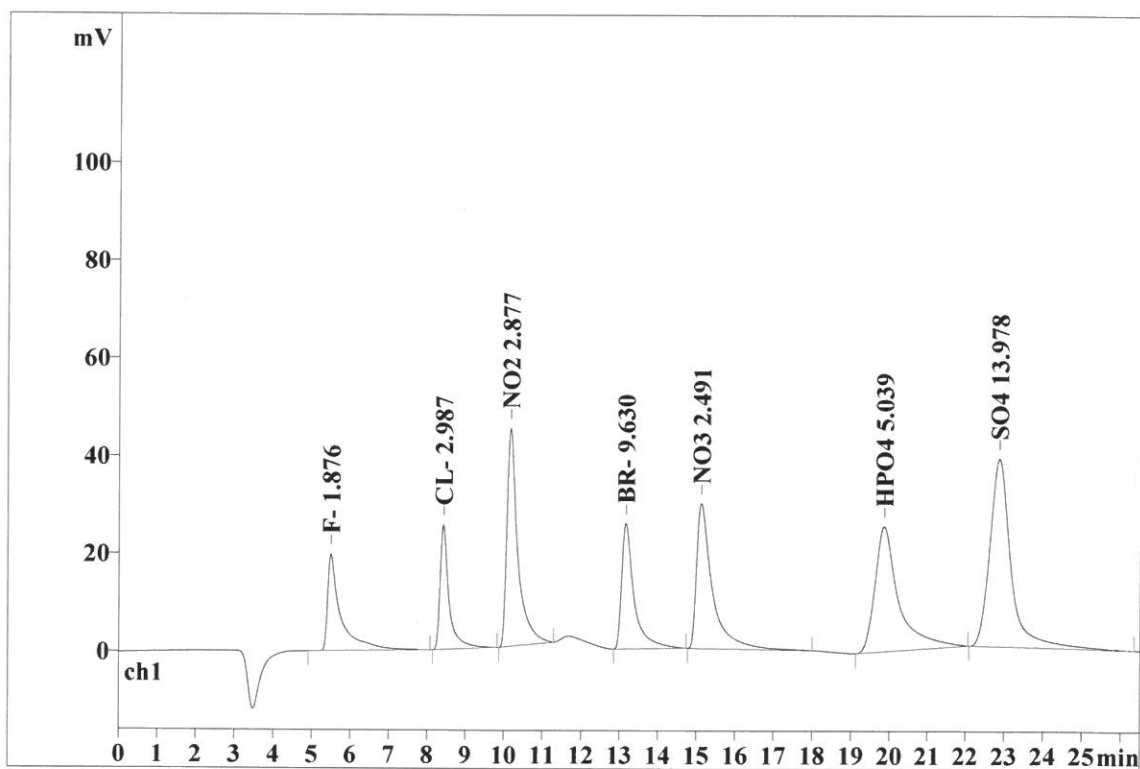

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.49	0.259	19.71	9.44	471.043	8.16
2	8.41	0.208	25.44	12.19	411.036	7.12
3	10.16	0.263	44.49	21.32	880.656	15.26
4	13.16	0.300	25.64	12.28	583.581	10.11
5	15.12	0.370	29.57	14.17	844.743	14.64
6	19.85	0.556	25.52	12.23	1105.625	19.16
7	22.87	0.526	38.35	18.37	1472.812	25.53
7	26.50	0.355	208.73	99.99	5769.496	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/26/2019 11:29:05 AM
Printed by: wet


Ident: K5111-09
Analysis from: 12/23/2019 1:54:37 PM
File: _2019-12-23_

Last save: 12/26/2019 11:28:08 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24079

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

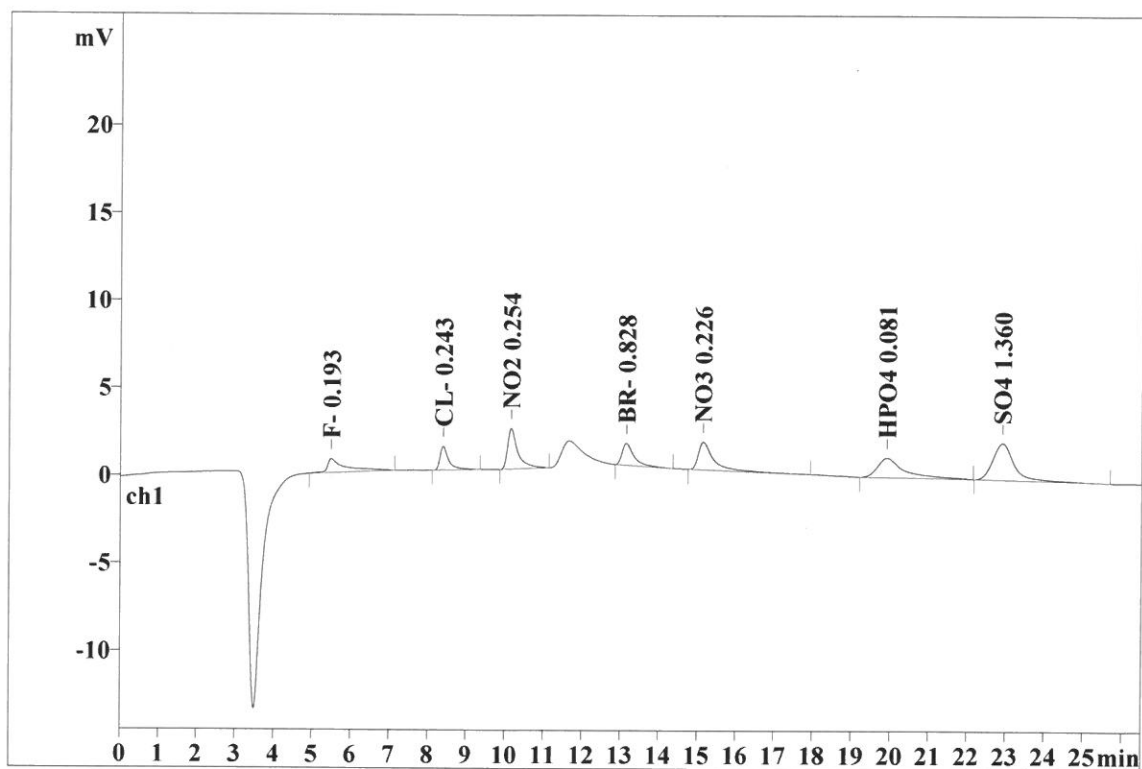

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.48	0.326	0.79	7.45	25.439	8.48
2	8.39	0.207	1.35	12.83	21.245	7.08
3	10.15	0.251	2.33	22.07	44.224	14.75
4	13.14	0.304	1.26	11.94	27.763	9.26
5	15.15	0.367	1.59	15.09	45.943	15.32
6	19.91	0.602	1.12	10.60	53.895	17.97
7	22.91	0.541	2.11	19.97	81.373	27.14
7	26.50	0.371	10.54	99.94	299.881	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/26/2019 11:30:46 AM
Printed by: wet


Ident: K5111-09RE
Analysis from: 12/23/2019 2:23:46 PM
File: _2019-12-23_

Last save: 12/26/2019 11:30:44 AM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24080

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

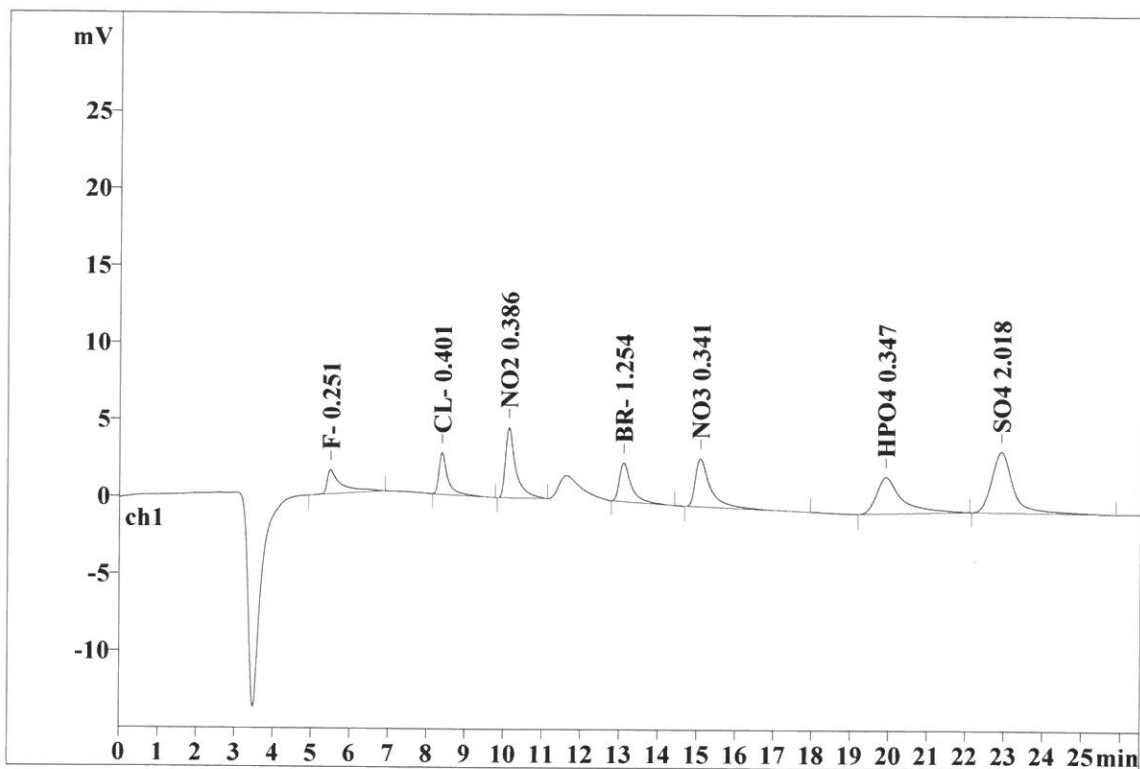

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.48	0.289	1.57	7.54	40.854	7.09
2	8.37	0.208	2.71	13.03	43.668	7.58
3	10.12	0.251	4.55	21.92	86.342	14.99
4	13.09	0.301	2.51	12.08	54.691	9.49
5	15.07	0.361	3.12	15.03	86.331	14.98
6	19.91	0.596	2.36	11.37	110.286	19.14
7	22.91	0.539	3.95	18.99	153.951	26.72
7	26.50	0.364	20.77	99.97	576.123	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/26/2019 11:30:57 AM
Printed by: wet


Ident: CCV
Analysis from: 12/23/2019 2:53:02 PM
File: _2019-12-23_

Last save: 12/23/2019 3:19:32 PM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24081

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

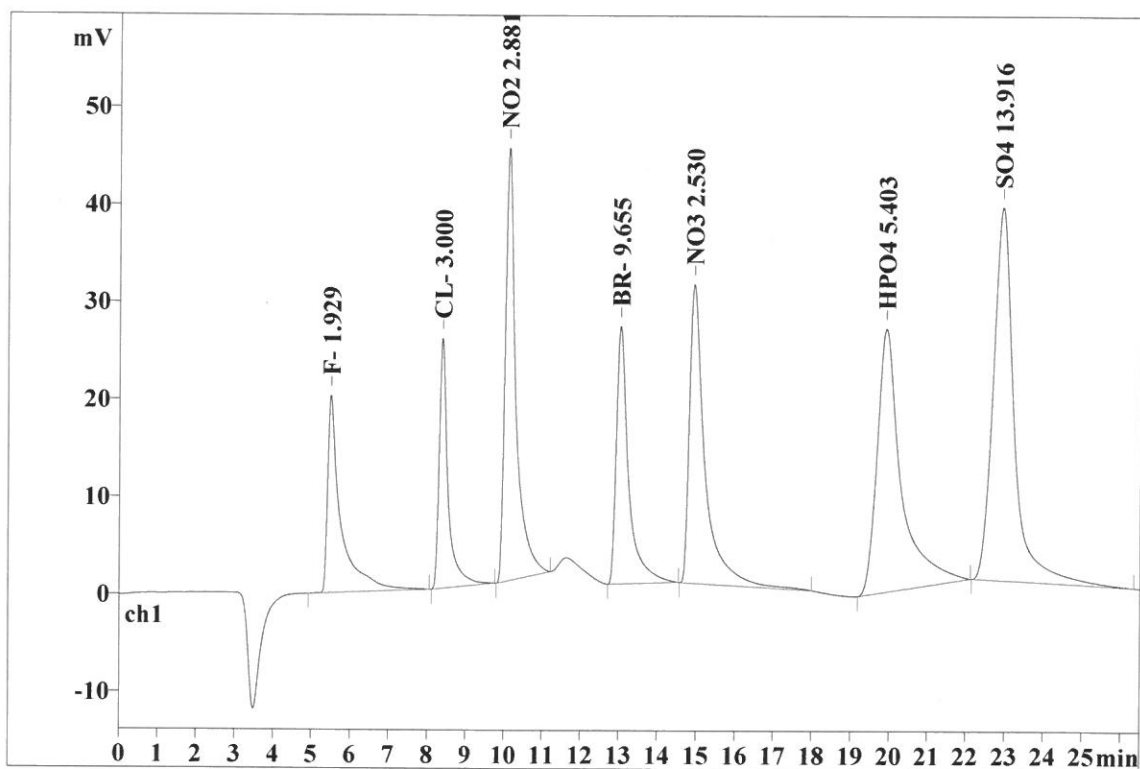

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.49	0.259	20.23	9.51	485.084	8.26
2	8.37	0.207	25.66	12.07	412.922	7.03
3	10.09	0.263	44.40	20.88	881.753	15.02
4	13.02	0.292	26.41	12.42	585.149	9.97
5	14.92	0.359	30.64	14.41	858.305	14.62
6	19.90	0.560	27.00	12.70	1182.705	20.14
7	22.92	0.525	38.28	18.00	1465.958	24.97
7	26.50	0.352	212.62	100.00	5871.876	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/26/2019 11:31:06 AM
Printed by: wet


Ident: CCB
Analysis from: 12/23/2019 3:22:11 PM
File: _2019-12-23_

Last save: 12/23/2019 3:48:41 PM

Method: AnionsIC2-121919.mtw
Run operator: wet
Analysis number: 24082

Last save: 12/20/2019 11:5

SAMPLE:
: CT/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

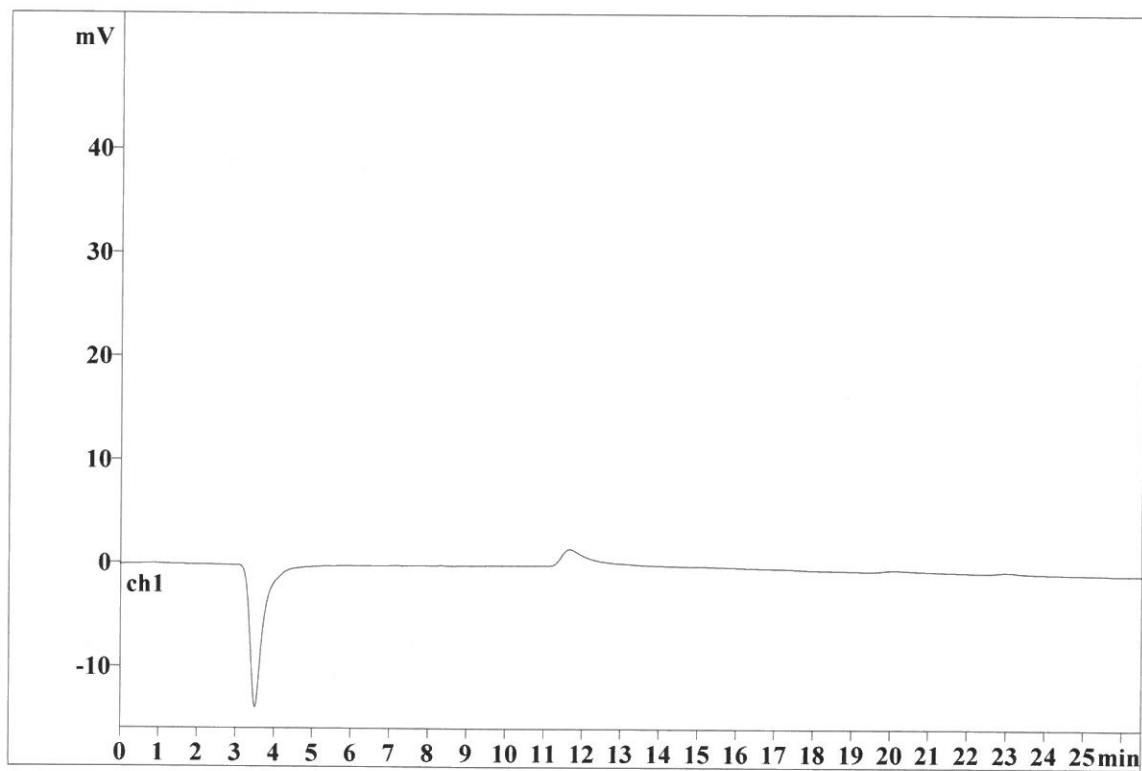

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD