

LB107006

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

1/2/2020 13:34

Test: ^{Reactive} Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.618	0.0	0.098	
ICB1	-0.454	0.0	0.003	
CCV1	242.722	0.0	0.242	
CCB1	-0.627	0.0	0.002	
PB125855BL	-0.700	0.0	0.002	
K6113-20	-0.701	0.0	0.002	
K6113-20DUP	-0.822	0.0	0.002	
K6472-07	-0.616	0.0	0.002	
K6474-02	-0.641	0.0	0.002	
K6474-04	-0.569	0.0	0.003	
K6479-05	-0.655	0.0	0.002	
CCV2	254.033	0.0	0.253	
CCB2	-0.778	0.0	0.002	

N	13
Mean	45.139
SD	94.1180
CV%	208.51

Aquakem v. 7.2AQ1

Results from time period:

Thu Jan 02 13:22:24 2020

Thu Jan 02 13:25:48 2020

AK

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	Cl P	-0.309	µg/l	1/2/2020 9:59:30	
5.OPPBCN	A	Reactive	Cl P	4.4378	µg/l	1/2/2020 9:59:31	
10PPBCN	A	Reactive	Cl P	9.7627	µg/l	1/2/2020 9:59:32	
50PPBCN	A	Reactive	Cl P	50.3017	µg/l	1/2/2020 9:59:33	
100PPBCN	A	Reactive	Cl P	99.7551	µg/l	1/2/2020 9:59:34	
250PPBCN	A	Reactive	Cl P	252.045	µg/l	1/2/2020 9:59:35	
500PPBCN	A	Reactive	Cl P	499.0067	µg/l	1/2/2020 9:59:36	
ICV1	S	Reactive	Cl P	96.6177	µg/l	1/2/2020 13:22:24	
ICB1	S	Reactive	Cl P	-0.4544	µg/l	1/2/2020 13:22:25	
CCV1	S	Reactive	Cl P	242.7224	µg/l	1/2/2020 13:22:26	
CCB1	S	Reactive	Cl P	-0.6271	µg/l	1/2/2020 13:22:27	
PB125855BL	S	Reactive	Cl P	-0.7002	µg/l	1/2/2020 13:22:28	
K6113-20	S	Reactive	Cl P	-0.7014	µg/l	1/2/2020 13:22:29	
K6113-20DUP	S	Reactive	Cl P	-0.8215	µg/l	1/2/2020 13:22:30	
K6472-07	S	Reactive	Cl P	-0.6164	µg/l	1/2/2020 13:22:31	
K6474-02	S	Reactive	Cl P	-0.6406	µg/l	1/2/2020 13:22:32	
K6474-04	S	Reactive	Cl P	-0.5692	µg/l	1/2/2020 13:22:33	
K6479-05	S	Reactive	Cl P	-0.6549	µg/l	1/2/2020 13:22:34	
CCV2	S	Reactive	Cl P	254.0333	µg/l	1/2/2020 13:25:47	
CCB2	S	Reactive	Cl P	-0.7776	µg/l	1/2/2020 13:25:48	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AK

Instrument ID : Konelab

1/2/2020 13:40


Test Total CN

Accepted 1/2/2020 10:05

Factor 1016
 Bias 0.003

Coeff. of det. 0.999972

Errors

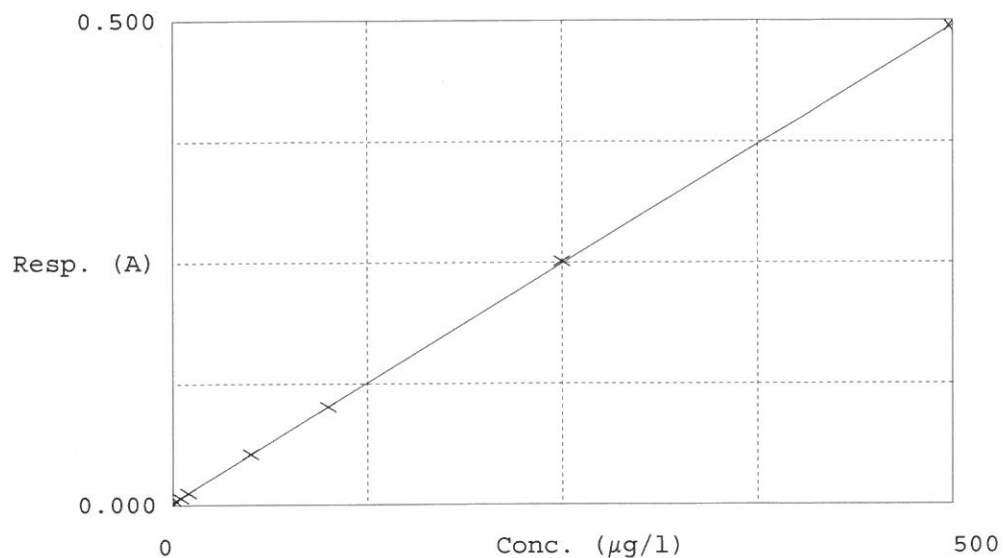

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.3090	0.0000	
2	5.0PPBCN	0.007	4.4378	5.0000	
3	10PPBCN	0.013	9.7627	10.0000	
4	50PPBCN	0.053	50.3017	50.0000	
5	100PPBCN	0.101	99.7551	100.0000	
6	250PPBCN	0.251	252.0450	250.0000	
7	500PPBCN	0.494	499.0067	500.0000	