


LB107015
INSTRUMENT ID C1

7471B

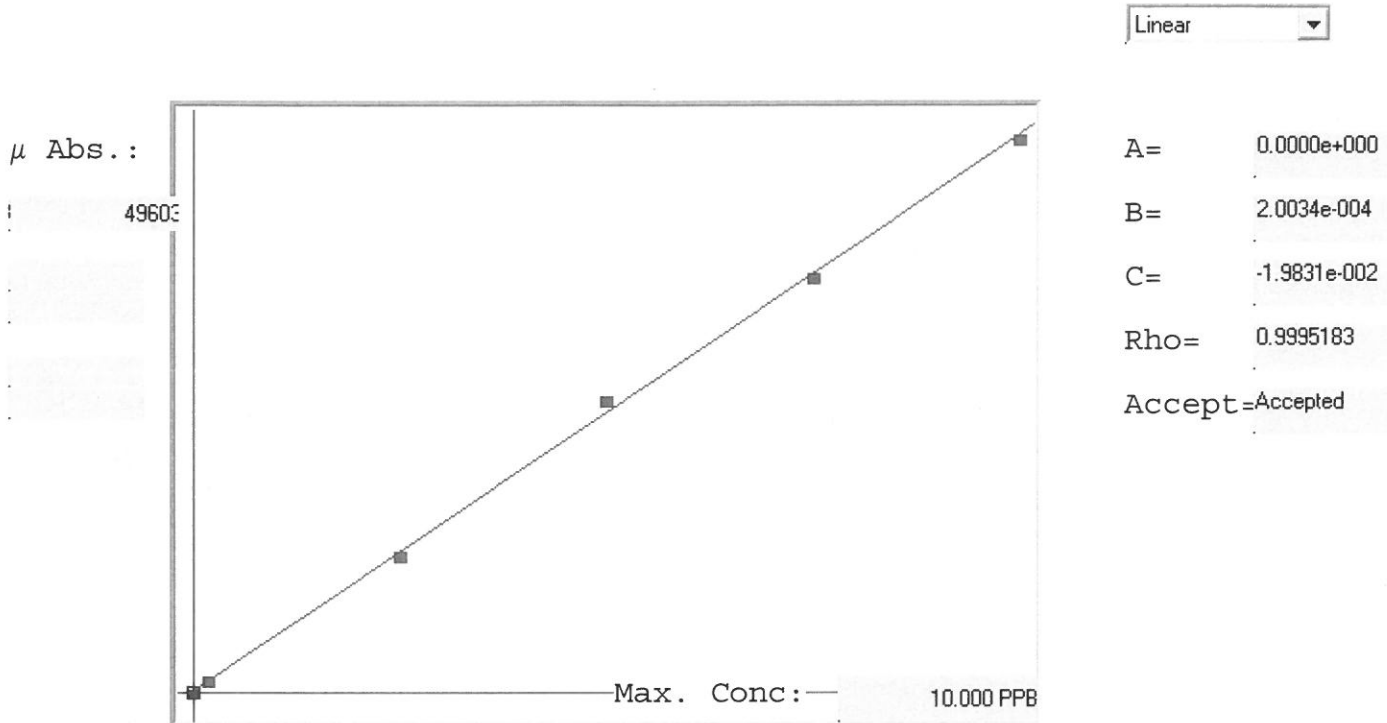

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.045	-0.045	-125	0.000	-125				
0.2	0.200	0.190	-0.010	1049	0.0 %	1049				
2.5	2.500	2.431	-0.069	12231	0.0 %	12231				
5.0	5.000	5.251	0.251	26309	0.0 %	26309				
7.5	7.500	7.455	-0.045	37311	0.0 %	37311				
10.0	10.000	9.918	-0.082	49603	0.0 %	49603				

LB107015 INSTRUMENT ID CV1

Method: 7471B		Operator: Admin		Date of Analysis: 03 Jan 2020 08:42:59					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	-125	-	0.0000	7471B	PPB	03 Jan 2020 08:48:45	S	Std
0.2 - 1	60.2	1049	-	0.2000	7471B	PPB	03 Jan 2020 08:51:01	S	Std
2.5 - 1	52.5	12231	-	2.5000	7471B	PPB	03 Jan 2020 08:53:19	S	Std
5.0 - 1	55.0	26309	-	5.0000	7471B	PPB	03 Jan 2020 08:55:35	S	Std
7.5 - 1	67.5	37311	-	7.5000	7471B	PPB	03 Jan 2020 08:57:51	S	Std
10.0 - 1	510.0	49603	-	10.0000	7471B	PPB	03 Jan 2020 09:00:07	S	Std
ICV49 - 1	ICV49	19778	3.9426	-	7471B	PPB	03 Jan 2020 09:02:53	U	SMPL
ICB49 - 1	ICB49	-43	-0.0284	-	7471B	PPB	03 Jan 2020 09:05:08	U	SMPL
CCV08 - 1	CCV08	26676	5.3245	-	7471B	PPB	03 Jan 2020 09:07:23	U	SMPL
CCB08 - 1	CCB08	-33	-0.0264	-	7471B	PPB	03 Jan 2020 09:09:37	U	SMPL
CRA - 1	CRA	1227	0.2260	-	7471B	PPB	03 Jan 2020 09:11:52	U	SMPL
HighStd - 1	HighStd	50577	10.1129	-	7471B	PPB	03 Jan 2020 09:14:07	U	SMPL
ChkStd - 1	ChkStd	36928	7.3784	-	7471B	PPB	03 Jan 2020 09:16:22	U	SMPL
PB125871BL - 1	PBS	-91	-0.0381	-	7471B	PPB	03 Jan 2020 09:18:39	U	SMPL
PB125871BS - 1	LCSS	20337	4.0546	-	7471B	PPB	03 Jan 2020 09:20:56	U	SMPL
K6113-16 - 1	OR-02-123119	9519	1.8872	-	7471B	PPB	03 Jan 2020 09:23:12	U	SMPL
K6113-16DUP - 1	OR-02-123119DUP	9435	1.8704	-	7471B	PPB	03 Jan 2020 09:25:28	U	SMPL
K6113-16MS - 1	OR-02-123119MS	32233	6.4378	-	7471B	PPB	03 Jan 2020 09:27:44	U	SMPL
K6113-16MSD - 1	OR-02-123119MSD	31189	6.2287	-	7471B	PPB	03 Jan 2020 09:30:01	U	SMPL
K6479-04 - 1	Q091-WC-01	6340	1.2503	-	7471B	PPB	03 Jan 2020 09:32:17	U	SMPL
CCV09 - 1	CCV09	25727	5.1344	-	7471B	PPB	03 Jan 2020 09:34:32	U	SMPL
CCB09 - 1	CCB09	-17	-0.0232	-	7471B	PPB	03 Jan 2020 09:36:48	U	SMPL
K6482-02 - 1	MC-123119-0-2-COMP-B6	47362	9.4688	-	7471B	PPB	03 Jan 2020 09:39:03	U	SMPL
K6482-04 - 1	MC-123119-2-5-COMP-B6	99093	19.8328	-	7471B	PPB	03 Jan 2020 09:41:18	U	SMPL
K6482-06 - 1	MC-123119-0-2-COMP-B4	7755	1.5338	-	7471B	PPB	03 Jan 2020 09:43:34	U	SMPL
K6482-08 - 1	MC-123119-2-5-COMP-B4	69584	13.9209	-	7471B	PPB	03 Jan 2020 09:45:51	U	SMPL
K6482-10 - 1	MC-123119-BD	5566	1.0953	-	7471B	PPB	03 Jan 2020 09:48:07	U	SMPL
K6484-44 - 1	40096-40103	26049	5.1989	-	7471B	PPB	03 Jan 2020 09:50:24	U	SMPL
K6484-46 - 1	40104-40111	48523	9.7014	-	7471B	PPB	03 Jan 2020 09:52:40	U	SMPL
K6484-48 - 1	40112-40120	39635	7.9208	-	7471B	PPB	03 Jan 2020 09:54:57	U	SMPL
K6484-50 - 1	30544-46-66	3588	0.6990	-	7471B	PPB	03 Jan 2020 09:57:15	U	SMPL
K6113-16LX5 - 1		1729	0.3266	-	7471B	PPB	03 Jan 2020 09:59:31	U	SMPL
CCV10 - 1	CCV10	25520	5.0929	-	7471B	PPB	03 Jan 2020 10:01:47	U	SMPL
CCB10 - 1	CCB10	-57	-0.0313	-	7471B	PPB	03 Jan 2020 10:04:02	U	SMPL
K6482-04DLX3 - 1		38157	7.6247	-	7471B	PPB	03 Jan 2020 10:06:17	U	SMPL
K6482-08DLX2 - 1		35533	7.0990	-	7471B	PPB	03 Jan 2020 10:08:33	U	SMPL
CCV11 - 1	CCV11	25854	5.1598	-	7471B	PPB	03 Jan 2020 10:10:48	U	SMPL
CCB11 - 1	CCB11	-45	-0.0288	-	7471B	PPB	03 Jan 2020 10:13:04	U	SMPL