

LB107043

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

1/6/2020 13:33

Test: ~~Total CN~~ *Reactive*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.279	0.0	0.100	
ICB1	0.121	0.0	0.002	
CCV1	240.652	0.0	0.249	
CCB1	0.186	0.0	0.002	
PB125906BL	0.057	0.0	0.002	
L1008-02	0.135	0.0	0.002	
L1008-02DUP	0.268	0.0	0.002	
L1009-02	0.075	0.0	0.002	
L1010-02	0.193	0.0	0.002	
CCV2	243.031	0.0	0.252	
CCB2	0.209	0.0	0.002	

N	11
Mean	52.746
SD	97.6996
CV%	185.23

Aquakem v. 7.2AQ1

Results from time period:

Mon Jan 06 12:12:03 2020

Mon Jan 06 13:31:27 2020

Sample Id	Sam/Ct	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.0198	µg/l	1/6/2020 13:01:31	
5.OPPBCN	A	Reactive CN	P	5.1087	µg/l	1/6/2020 13:01:32	
10PPBCN	A	Reactive CN	P	9.5249	µg/l	1/6/2020 13:01:33	
50PPBCN	A	Reactive CN	P	49.828	µg/l	1/6/2020 13:01:34	
100PPBCN	A	Reactive CN	P	99.8517	µg/l	1/6/2020 13:01:35	
250PPBCN	A	Reactive CN	P	251.2233	µg/l	1/6/2020 13:01:36	
500PPBCN	A	Reactive CN	P	499.4436	µg/l	1/6/2020 13:01:37	
ICV1	S	Reactive CN	P	95.279	µg/l	1/6/2020 13:31:17	
ICB1	S	Reactive CN	P	0.1209	µg/l	1/6/2020 13:31:18	
CCV1	S	Reactive CN	P	240.6522	µg/l	1/6/2020 13:31:19	
CCB1	S	Reactive CN	P	0.1858	µg/l	1/6/2020 13:31:20	
PB125906BL	S	Reactive CN	P	0.0568	µg/l	1/6/2020 13:31:21	
L1008-02	S	Reactive CN	P	0.135	µg/l	1/6/2020 13:31:22	
L1008-02DUP	S	Reactive CN	P	0.2677	µg/l	1/6/2020 13:31:23	
L1009-02	S	Reactive CN	P	0.0755	µg/l	1/6/2020 13:31:24	
L1010-02	S	Reactive CN	P	0.1934	µg/l	1/6/2020 13:31:25	
CCV2	S	Reactive CN	P	243.0305	µg/l	1/6/2020 13:31:26	
CCB2	S	Reactive CN	P	0.2092	µg/l	1/6/2020 13:31:27	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

1/6/2020 13:04

Test Total CN


Accepted 1/6/2020 13:04

Factor 973.4

Bias 0.002

Coeff. of det. 0.999990

Errors

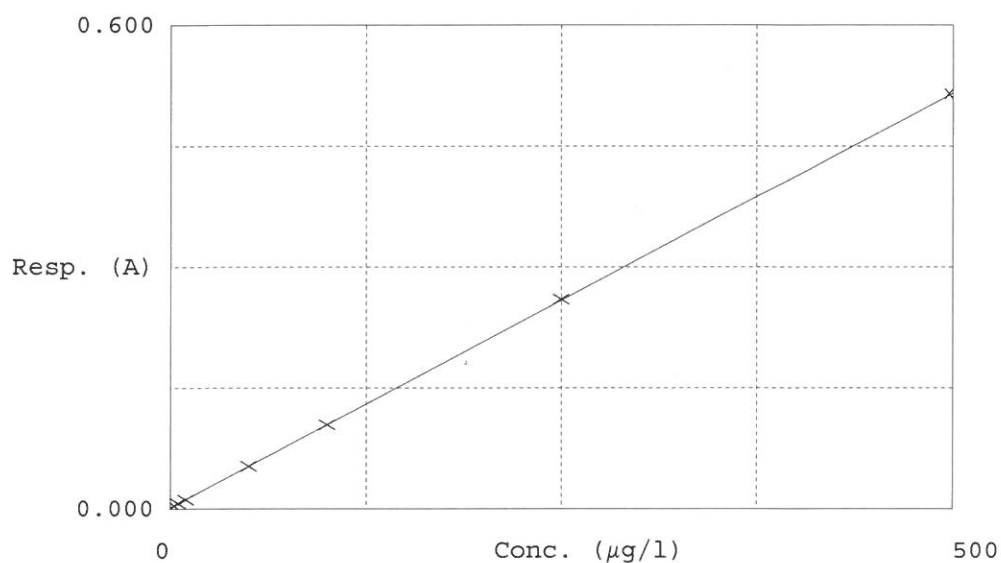

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.0198	0.0000	
2	5.0PPBCN	0.007	5.1087	5.0000	
3	10PPBCN	0.012	9.5249	10.0000	
4	50PPBCN	0.053	49.8280	50.0000	
5	100PPBCN	0.104	99.8517	100.0000	
6	250PPBCN	0.260	251.2233	250.0000	
7	500PPBCN	0.515	499.4436	500.0000	