


LB107057
INSTRUMENT ID CV1

ISM02.4

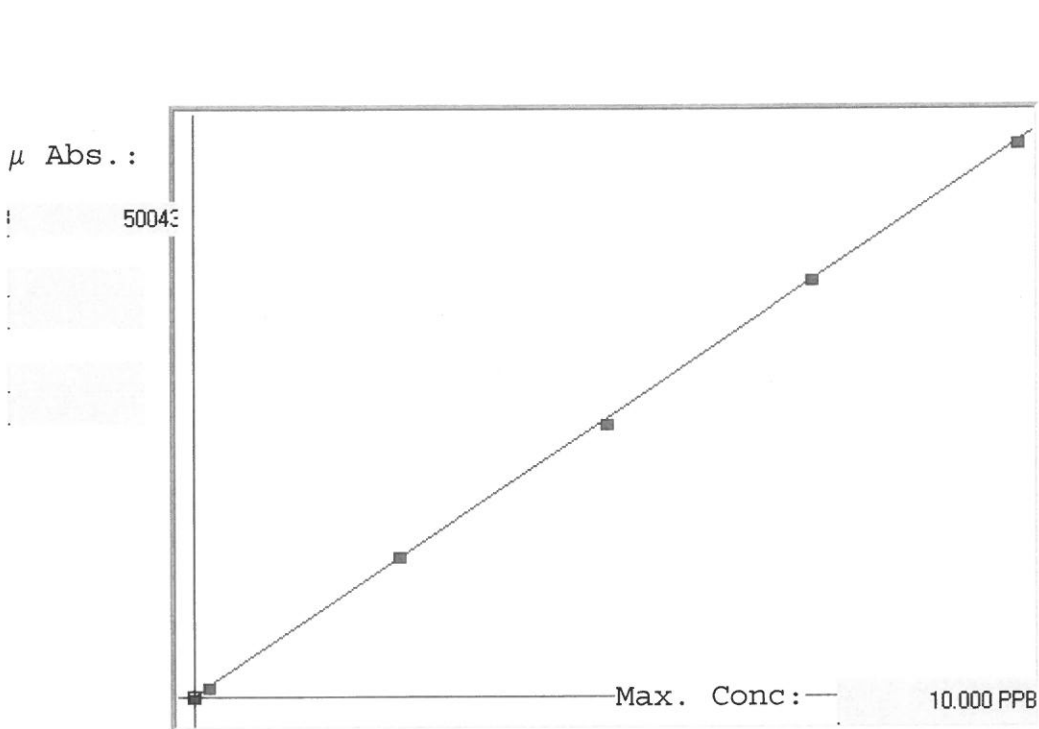

Linear

A= 0.0000e+000

B= 1.9973e-004 slope

C= -1.9996e-003 y-intercept

Rho= 0.9999411

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.00	0.000	-0.012	-0.012	-48	0.000	-48					
0.05	0.050										
0.20	0.200	0.201	0.001	1018	0.0 %	1018					0
2.50	2.500	2.550	0.050	12779	0.0 %	12779					2
5.00	5.000	4.927	-0.073	24679	0.0 %	24679					-1
7.50	7.500	7.540	0.040	37761	0.0 %	37761					0
10.0	10.000	9.993	-0.007	50043	0.0 %	50043					0

6/10/20

LB107057
INSTRUMENT ID CV1

Sample ID	Extended II μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	
0 S0	-48	-	0	ISM02.4	PPB	1/7/2020 8:10	Std	
0.2 S0.2	1018	-	0.2	ISM02.4	PPB	1/7/2020 8:12	Std	
2.5 S2.5	12779	-	2.5	ISM02.4	PPB	1/7/2020 8:14	Std	
5 S5.0	24679	-	5	ISM02.4	PPB	1/7/2020 8:16	Std	
7.5 S7.5	37761	-	7.5	ISM02.4	PPB	1/7/2020 8:19	Std	
10 S10.0	50043	-	10	ISM02.4	PPB	1/7/2020 8:24	Std	
ICV052	ICV052	18724	3.7377	-	ISM02.4	PPB	1/7/2020 8:27	SMPL
ICB052	ICB052	-50	-0.012	-	ISM02.4	PPB	1/7/2020 8:29	SMPL
CCV019	CCV019	24626	4.9165	-	ISM02.4	PPB	1/7/2020 8:31	SMPL
CCB019	CCB019	-55	-0.013	-	ISM02.4	PPB	1/7/2020 8:33	SMPL
PB125919E	PBW919	-20	-0.006	-	ISM02.4	PPB	1/7/2020 8:36	SMPL
K6445-07	X2K07	17080	3.4093	-	ISM02.4	PPB	1/7/2020 8:46	SMPL
K6445-08	X2K07D	17098	3.4129	-	ISM02.4	PPB	1/7/2020 8:48	SMPL
K6445-09	X2K07S	21834	4.3588	-	ISM02.4	PPB	1/7/2020 8:50	SMPL
CCV020	CCV020	24116	4.8146	-	ISM02.4	PPB	1/7/2020 8:56	SMPL
CCB020	CCB020	-87	-0.0194	-	ISM02.4	PPB	1/7/2020 8:58	SMPL