

LB107062

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

Instrument ID : Konelab

1/7/2020 13:06

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.555	0.0	0.098	
ICB1	0.794	0.0	0.003	
CCV1	236.232	0.0	0.244	
CCB1	0.706	0.0	0.003	
PB125933BL	0.562	0.0	0.002	
PB125933BS	96.386	0.0	0.101	
LOWPB125933	10.487	0.0	0.013	
HIGHPB125933	486.199	0.0	0.501	
L1017-01	1.607	0.0	0.003	
L1017-01DUP	1.352	0.0	0.003	
L1017-01MS	29.098	0.0	0.032	
L1017-01MSD	27.705	0.0	0.030	
L1039-01	0.822	0.0	0.003	
L1039-05	1.167	0.0	0.003	
CCV2	252.440	0.0	0.261	
CCB2	0.652	0.0	0.002	

N	16
Mean	77.485
SD	136.5364
CV%	176.21

Aquakem v. 7.2AQ1

Results from time period:

Tue Jan 07 12:57:41 2020

Tue Jan 07 13:02:32 2020

AL

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.1276	µg/l	1/7/2020 9:18:35	
5.OPPBCN	A	Total CN	P	5.325	µg/l	1/7/2020 9:18:36	
10PPBCN	A	Total CN	P	10.1222	µg/l	1/7/2020 9:18:37	
50PPBCN	A	Total CN	P	49.6672	µg/l	1/7/2020 9:18:38	
100PPBCN	A	Total CN	P	100.2307	µg/l	1/7/2020 9:18:39	
250PPBCN	A	Total CN	P	249.0916	µg/l	1/7/2020 9:18:40	
500PPBCN	A	Total CN	P	500.4357	µg/l	1/7/2020 9:18:41	
ICV1	S	Total CN	P	93.5554	µg/l	1/7/2020 12:57:41	
ICB1	S	Total CN	P	0.7939	µg/l	1/7/2020 12:57:42	
CCV1	S	Total CN	P	236.2323	µg/l	1/7/2020 12:57:43	
CCB1	S	Total CN	P	0.7064	µg/l	1/7/2020 12:57:44	
PB125933BL	S	Total CN	P	0.5624	µg/l	1/7/2020 12:57:45	
PB125933BS	S	Total CN	P	96.3858	µg/l	1/7/2020 12:57:46	
LOWPB125933	S	Total CN	P	10.4875	µg/l	1/7/2020 12:57:47	
HIGHPB125933	S	Total CN	P	486.1992	µg/l	1/7/2020 12:57:48	
L1017-01	S	Total CN	P	1.6069	µg/l	1/7/2020 12:57:49	
L1017-01DUP	S	Total CN	P	1.3524	µg/l	1/7/2020 12:57:50	
L1017-01MS	S	Total CN	P	29.0978	µg/l	1/7/2020 12:57:51	
L1017-01MSD	S	Total CN	P	27.7054	µg/l	1/7/2020 13:02:28	
L1039-01	S	Total CN	P	0.822	µg/l	1/7/2020 13:02:29	
L1039-05	S	Total CN	P	1.1666	µg/l	1/7/2020 13:02:30	
CCV2	S	Total CN	P	252.4399	µg/l	1/7/2020 13:02:31	
CCB2	S	Total CN	P	0.6519	µg/l	1/7/2020 13:02:32	

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

Instrument ID : Konelab

1/7/2020 13:32

Test Total CN


Accepted 1/7/2020 9:25

Factor 973.5

Bias 0.002

Coeff. of det. 0.999994

Errors

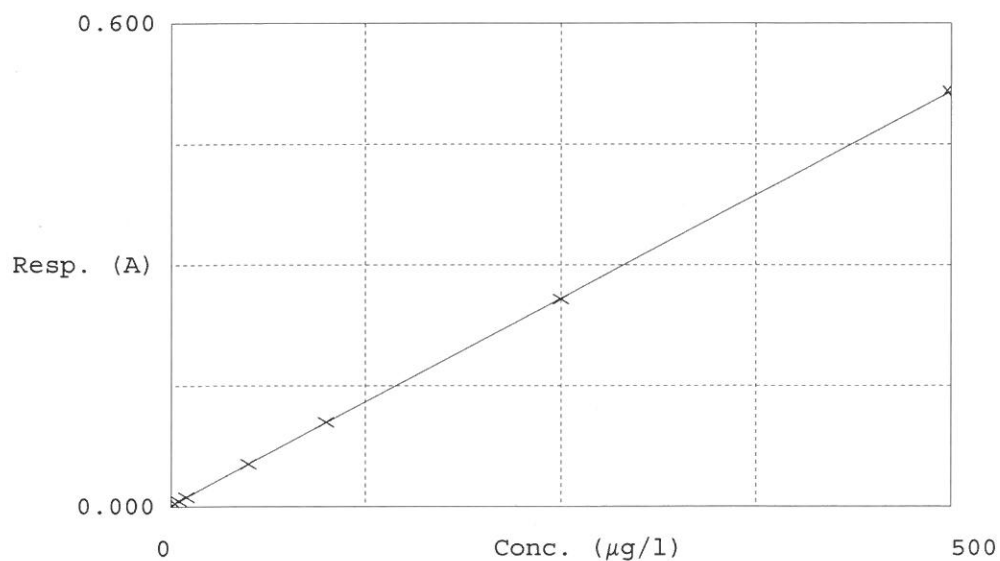

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.1276	0.0000	
2	5.0PPBCN	0.007	5.3250	5.0000	
3	10PPBCN	0.012	10.1222	10.0000	
4	50PPBCN	0.053	49.6672	50.0000	
5	100PPBCN	0.105	100.2307	100.0000	
6	250PPBCN	0.258	249.0916	250.0000	
7	500PPBCN	0.516	500.4357	500.0000	